



Automated Hematology Analyzer
XN-L series

XN-530/XN-430 /XN-330

General Information

This manual provides important safety information and specifications of the instrument.
Read this manual before using the instrument.

The following manuals are provided as Instructions for Use:

- General Information
- Basic Operation
- Troubleshooting

Sysmex Corporation

KOBE, JAPAN

Code No. AC044589 en-eu
PRINTED IN JAPAN
Date of Last Revision: 04/2020
Software Version: Ver. 5 onwards

Revision History

06/2016

Initial issue

Software version: Ver. 5

02/2017

Software version: Ver. 5

05/2017

Software version: Ver. 5

01/2018

Software version: Ver. 5

08/2018

Software version: Ver. 5

06/2019

Software version: Ver. 5

04/2020

Software version: Ver. 5

Changes are listed below:

Revised section	Page
1.3 Reportable parameters	10
6.2 Accessories	75
8.1.2 [WDF] service data	89
8.2.1 WBC research parameters	92
Addition of descriptions related to XN-530 and XN-430	Throughout the manual

Table of Contents

Revision History	3
Chapter 1 Introduction	7
1.1 Intended use	9
1.2 Overview of the system	9
1.3 Reportable parameters	10
1.4 About the manuals	11
1.5 Symbols used in the manuals	12
1.6 Symbols related to the products	13
1.7 Trademarks	14
Chapter 2 Safety Information	15
2.1 General information	15
2.2 Installation	16
2.3 Electromagnetic compatibility (EMC)	17
2.4 Avoiding infection	18
2.5 Handling of reagents and quality control materials	18
2.6 Laser	19
2.7 Maintenance	19
2.8 Disposal of materials	19
2.9 Operators	20
2.10 Computer viruses	20
2.11 Use of other software	21
2.12 Markings on the instrument	21
Chapter 3 Part Names and Functions	29
3.1 Analyzer	29
3.2 Monitor (XN-530)	36
Chapter 4 Installation	37
4.1 Preparing for installation	37
4.2 Installation	38
Chapter 5 Instrument Specifications	41
5.1 Specifications	41
5.2 System limitations	57
5.3 Supported sample tubes and sampler adapter	60
5.4 Barcode labels (XN-530)	63
5.5 ID barcode specifications	64
5.6 Functional descriptions	66
Chapter 6 Supplies, Accessories, and Options	75
6.1 Supplies	75
6.2 Accessories	75
6.3 Options	76

Chapter 7	Reagents	77
7.1	General information	77
7.2	List of specified reagents	77
7.3	CELLPACK DCL	78
7.4	CELLPACK DST	79
7.5	SULFOLYSER	80
7.6	Lysercell WDF	81
7.7	Fluorocell WDF	82
7.8	CELLCLEAN AUTO	83
7.9	Control blood (XN-L CHECK)	84
7.10	Calibrator (XN CAL)	85
Chapter 8	Service Data and Research Parameters	87
8.1	Checking service data	87
8.2	Checking research parameters	91
Index		93

Chapter 1 Introduction

Thank you for purchasing the Automated Hematology Analyzer XN-L series.
Please read this manual carefully before operating this product.
Keep this manual in a safe place for future reference.



Note:

- Data generated by the XN-L series is not intended to replace professional judgment in the determination of a diagnosis or in monitoring patient therapy.
- Operate the instrument as instructed. Reliability of test results cannot be guaranteed if there are any deviations from the instructions in this manual. If the instrument fails to function properly as a result of either the user's operation not specified in the manual or the user's utilization of a program not specified by Sysmex, the product warranty would not apply.

Contact Addresses



Sysmex Corporation
1-5-1 Wakinojima-Kaigandori, Chuo-ku, Kobe 651-0073, Japan

Authorized Representative / Importer to EU

Europe, Middle East and Africa



Sysmex Europe GmbH
Bornbarch 1, 22848 Norderstedt, Germany
Phone: +49 40 5 27 26-0 / Fax: +49 40 5 27 26-100

Authorized Representatives

Americas

Sysmex America, Inc.
577 Aptakisic Road, Lincolnshire, IL 60069, U.S.A.
Phone: +1-224-543-9500 / Fax: +1-224-543-9505

Asia-Pacific

Sysmex Asia Pacific Pte Ltd.
9 Tampines Grande #06-18 Singapore 528735
Phone: +65-6221-3629 / Fax: +65-6221-3687

Ordering of Supplies and Replacement Parts

If you need to order supplies or replacement parts, please contact your local Sysmex representative.

Service and Maintenance

Please contact the Service Department of your local Sysmex representative.



The system described in this manual is marked with a CE-mark which confirms the compliance with the essential requirements of the following European Directives:

98/79/EC on in vitro diagnostic medical devices

2011/65/EU on the restriction of the use of certain hazardous substances in electrical and electronic equipment

2014/53/EU relating to the making available on the market of radio equipment

www.systemex-europe.com/ifu



The system described in this manual is compliant with the European In-Vitro Diagnostic (IVD) Directive and additionally marked with an EAC-mark which confirms the compliance with applicable Technical Regulations of Eurasian Economic Union.

1.1 Intended use

The XN-L series are automated hematology analyzers for in vitro diagnostic use in clinical laboratories. Only human blood or control blood should be run. Any other use is regarded as non-specified.


Use only the reagents and cleaning fluids indicated in this manual.

If the instrument fails to function properly as a result of either the user's operation not specified in the manual or the user's utilization of a program not specified by Sysmex, the product warranty does not apply.


1.2 Overview of the system

This instrument is a hematology analyzer for in vitro diagnostic use in screening patient populations found in clinical laboratories.

This instrument enables quantitative, identification, and existence ratio analysis of tangible components of blood (red blood cells, white blood cells, platelets and other cells) by means of electrical impedance, laser light scattering and fluorescent labeling.

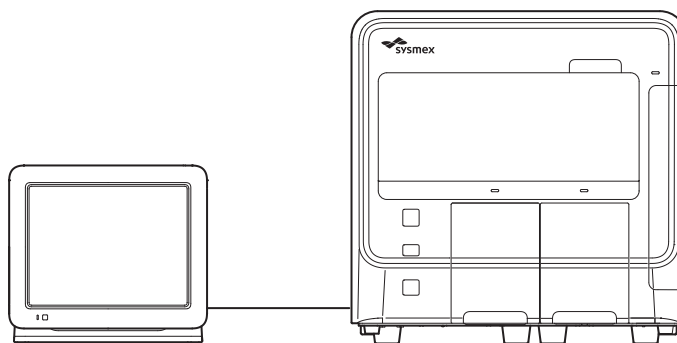

XN-530

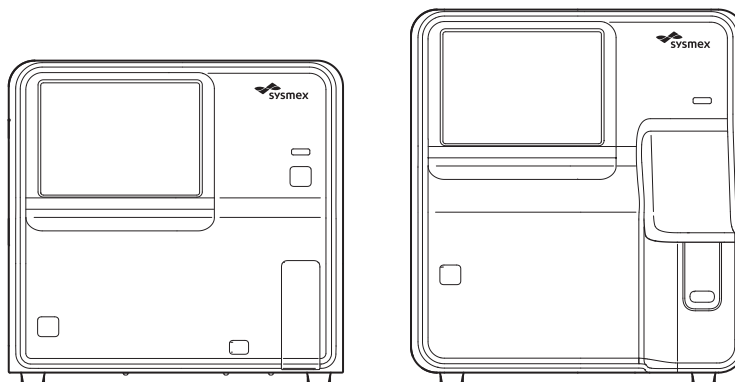

XN-430

XN-330

		XN-530 Sampler analysis type	XN-430 Closed analysis type	XN-330 Open analysis type
Channels	WDF		✓	
	RBC/PLT		✓	
	HGB		✓	
Analysis mode	[Whole Blood]		✓	
	[Pre-Dilution]		✓	

1.3 Reportable parameters

This instrument reports the following parameters.

● Reportable parameters

[Whole Blood] mode / [Pre-Dilution] mode	
Detector/Channel	Parameter
WDF	WBC, NEUT#, LYMPH#, MONO#, EO#, BASO#, NEUT%, LYMPH%, MONO%, EO%, BASO%, IG#, IG%
RBC/PLT	RBC, HCT, MCV ^{*1} , MCH ^{*1} , MCHC ^{*1} , PLT, RDW-SD ^{*2} , RDW-CV ^{*2} , MicroR ^{*3,4} , MacroR ^{*3,4} , PDW ^{*2} , MPV ^{*1} , P-LCR ^{*2} , PCT ^{*2}
HGB	HGB

*1 Parameter calculated from an equation. For details, see the following.

(►P.71 "Chapter 5: 5.6.3 Reportable parameters and channels")

*2 Parameters calculated from an equation from the distribution. For details, see the following.

(►P.71 "Chapter 5: 5.6.3 Reportable parameters and channels")

*3 Parameters calculated from an equation from the distribution.

*4 Analysis is not possible in [Pre-Dilution] mode.

1.4 About the manuals

1.4.1 List of manuals

The following manuals are provided with this instrument.

	Type	Description
Instructions for Use	General Information (this manual)	This manual provides important safety information and specifications of the instrument. Read this manual before using the instrument.
	Basic Operation	Read this manual to operate the instrument. The explanations in this manual assume that you have already read "General Information".
	Troubleshooting	Read this manual when you encounter a problem, and to perform instrument maintenance. The explanations in this manual assume that you have already read "General Information".

1.4.2 Points to note about the manuals

- You may not reprint the contents of the manuals in whole or in part without permission.
- The names of patients, doctors, etc., mentioned in the manuals do not represent actual people in any way.
- Images in these instructions for use related to the product are for illustration purposes only and may not exactly match with what is found on the product itself.
- While we have taken all possible precautions to ensure quality in the content of this manual, please contact the Service Department of your local Sysmex representative if you find any errors or omissions.

1.5 Symbols used in the manuals



Risk of infection

Indicates the presence of a biohazardous material or condition.



Warning!

High risk. Ignoring this warning could result in personal injury to the operator.



Caution!

Average risk. Ignoring this warning could result in property damage. Intended to avoid damage and incorrect measuring results.



Caution, Hot!

Indicates risk of burns and other injuries if the warning is not observed.



Caution!

Failure to observe this warning may result in instrument damage due to electrostatic discharge from your body.



Information



















Minor risk. Considerations that should be observed when operating this instrument.



Note:

Background information and practical tips.

1.6 Symbols related to the products

	In vitro diagnostic medical device		Concentrated reagent
	Manufacturer		Keep away from sunlight
	Authorized representative in the European Community		Use no hooks
	Consult instructions for use		This way up
	Temperature limitation		Keep dry
	Biological risks		Stacking limit by number
	Use by		Fragile; handle with care
	Batch code		Corrugated recycles
	Catalogue number		By prescription only* * In compliance with U.S. FDA requirements

1.7 Trademarks

- Sysmex is a trademark of SYSMEX CORPORATION, Japan.
- CELLPACK, CELLCLEAN, Fluorocell, SULFOLYSER, and Lysercell are trademarks of SYSMEX CORPORATION.
- ISBT128 (International Society of Blood Transfusion) is copyrighted by and is used under License Agreement with ICCBBA, Inc.
- Windows is a trademark or registered trademark of Microsoft Corporation in the United States and other countries.
- Other company names and product names in the manuals are the registered trademarks or trademarks of their respective owners.

The fact that a trademark is not explicitly indicated in this manual does not authorize its use.

TM and ® are not explicitly indicated in the manuals.

Chapter 2 Safety Information

This chapter explains precautions for safe use of this instrument.

2.1 General information



Warning!

- Keep your hair, fingers and clothing away from the instrument that are in operation. You may get injured if caught in the instrument.
- Do not spill blood samples or reagents into the instrument, or get any metals such as staples or clips, inside the instrument.
Doing so could cause a short-circuit and a smoke emission.
- The operator should not touch any electrical circuitry inside the cover.
The risk of electrical shock is especially high when your hands are wet.
- The instrument must not be connected to a power outlet other than that specified on the rating plate.
Please note that the instrument must be grounded.
Failure to do so may result in fire or electrical shock.
- Avoid damage to the power cable: do not place any heavy object on the power cable or pull on it.
Doing so may cause fire or shock due to an electrical short or break in the wiring.
- In the unlikely event that the instrument emits an unusual odor or smoke, immediately turn OFF the main switch and unplug the power cable. Then contact your Sysmex service representative.
Continued use of the instrument in such conditions could result in fire, electrical shock or personal injury.



Caution!

- When handling the sampler adapter (XN-530) and sample tubes, take care not to spill the sample.
- Do not lean against the instrument.
The resulting impact could damage the instrument or cause it to tip over.
- For maintenance tasks that require a washing solution, always use CELLCLEAN AUTO. If CELLCLEAN AUTO is not used, the instrument will not be cleaned sufficiently and problems may result.
 - * It is also possible to use CELLCLEAN in place of CELLCLEAN AUTO. In this case, use 4 mL of CELLCLEAN manually dispensed into a clean sample tube. As this manual assumes that CELLCLEAN AUTO is used, substitute "CELLCLEAN" whenever "CELLCLEAN AUTO" appears.
- Do not analyze coagulated blood.



cTÜVus mark indicates that the equipment is tested and certified to comply with the electrical and fire safety regulations controlled by the US and Canadian governments.

Those tests were conducted thoroughly by TÜV Rheinland that is accredited as a Nationally Recognized Testing Laboratory (NRTL) by OSHA (The Occupational Safety and Health Administration) in the United States, and by SCC (Standards Council of Canada) in Canada.

2.2 Installation



Warning!

- Your Sysmex technical representative will unpack, install, and test initial operation of the instrument.
- This instrument must not be connected to a power outlet rated at anything other than specified on the rating plate. Please note that the instrument must be grounded. Failure to do so may result in fire or electrical shock.
- Switch OFF the power supply before connecting any peripheral devices (host computer, printer, etc.). Failure to do so may result in electrical shock or damage to instrument. In addition, an abnormal stop may occur if a device is connected while the instrument is running.



Caution!

- Install in a location where water will not splash or spray onto the instrument.
- Install in a location where the instrument will be protected from high temperature, humidity, dust and direct sunlight.
- Do not install in a location subject to vibration.
- Do not subject the instrument to intense shock or vibration.
- Install the instrument in a well-ventilated place.
- Avoid installing the instrument near equipment that emits electrical interference, such as a radio or centrifuge.
- Do not install the instrument near an area where chemicals are stored or gases are emitted.
- Do not use the instrument in a location where electroconductive gases, flammable gases, or anesthetics that contain oxygen, hydrogen, or other flammable gases are present.
- Install the instrument indoors.
The instrument is intended for indoor use only.
- Place the reagent container at a level no more than 1 meter above or below the bottom of the analyzer. Do not place reagents on top of the instrument.
- The instrument uses the common reagents for the XN series; however, a different spout set is used. Be sure to use the correct spout set.

2.3 Electromagnetic compatibility (EMC)

This instrument complies with the following IEC (EN) standards:

- IEC61326-2-6:2005 (EN61326-2-6:2006)
Electrical equipment for measurement, control and laboratory use - EMC requirements
- EMI (Electromagnetic Interference) For this standard the requirements of class A are fulfilled.
- EMS (Electromagnetic Susceptibility) For this standard the minimum requirements with regards to susceptibility are fulfilled.
- This equipment has been designed and tested to CISPR11 Class A. In a domestic environment it may cause a radio interference, in which case, you may need to take measures to mitigate the interference. The electromagnetic environment should be evaluated prior to operation of the device.
Do not use this device in close proximity to sources of strong electromagnetic radiation (e.g. unshielded intentional RF sources), as these may interfere with the proper operation.

This instrument includes an RFID (Radio-Frequency Identification Device) module.

- RFID device: PC-1160002
- Intended use: This RFID module is an electromagnetic induction type non-contact IC can read and write RFID tag data.
- Frequency band: 13.56 MHz
- Maximum radio-frequency power: 23.9 dBuV/m at 3 m (QP)



Caution!

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

2.4 Avoiding infection



Risk of infection

- When performing any task on the instrument, such as testing, maintenance, preparation, or post processing, be sure to wear adequate personal protective equipment, such as protective gloves, a protective mask, protective eyewear, and a lab coat. Wash your hands with antiseptic solution after completing the task. There is a risk of infection.
- Be sure to connect the instrument's drain tubing to a waste fluid tank at the facility or other dedicated waste container.
If connecting the tubing to a waste fluid tank at the facility, use a tank with a nipple to which the drain tubing can be attached or a tank with other means of securing the tubing in place so as to avoid the risk of waste fluid spillage. In addition, exercise care so as to avoid such spillage, for example by regularly verifying that the tube remains properly secured in place.
- Never touch waste, or parts that have come in contact with waste, with your bare hands.
If you inadvertently come in contact with potentially infectious materials or surfaces, immediately rinse the skin with large amounts of water, and then follow your laboratory's prescribed cleaning and decontamination procedures.
- Use appropriate care when handling samples and quality control materials.
In the event that an infectious material gets in the eyes or an open wound, rinse with large amounts of water and seek immediate medical attention.
- Exercise caution when handling waste fluid. If waste fluid comes in contact with your body or clothes, wash thoroughly.
- Do not dispose of waste fluid while analysis is in progress.

2.5 Handling of reagents and quality control materials



Warning!

- CELLPACK diluent is an electrical conductor. If diluent is spilled inadvertently near electrical cables or appliances, there is a risk of electrical shock. Switch OFF the instrument, unplug the power cable, and wipe off the liquid.
- Be sure to use CELLCLEAN AUTO only when rinsing the inside of the instrument.
- CELLCLEAN AUTO contains sodium hypochlorite.
If CELLCLEAN AUTO comes in contact with the instrument's surface, it may corrode its finish. Immediately wipe off with a damp cloth.



Caution!

Follow the directions on the reagent container.

For other cautionary points, see Chapter 7.

(►P.77 "Chapter 7 Reagents")

2.6 Laser



Warning!

The analyzers have a semiconductor laser unit that is located inside the instrument. To avoid physical risk of injury from the laser, access is limited to authorized Sysmex technical representative.

2.7 Maintenance



Information

When performing maintenance, use only the tools specially authorized by Sysmex.

2.8 Disposal of materials

2.8.1 Waste Disposal



Risk of infection

After becoming waste at end-of-life, this instrument and its accessories are regarded as infectious. They are therefore exempted from EU directive 2012/19/EU (Waste Electrical and Electronic Equipment Directive) and may not be collected by public recycling to prevent possible risk of infection of personnel working at those recycling facilities.



Warning!

- Do not dispose the instrument, accessories and consumables via public recycling!
- Incineration of contaminated parts is recommended!
- Contact your local Sysmex service representative and receive further instructions for disposal!
Follow local legal requirements at all times.



Caution!

Waste effluents from the instrument may contain dangerous substances and decision about disposal only has to be made by local water authority.



This symbol is affixed by the requirement by Article 14. (4) of the WEEE Directive (2012/19/EU), and indicates the waste end-of-life equipment should not be disposed as unsorted municipal waste and such equipment shall be collected separately.

2.8.2 Decontamination



Warning!

Before decontaminating the instrument, be sure to turn off the power supply and unplug the power cord. This is necessary to avoid the risk of electric shock. When cleaning the instrument, always wear adequate personal protective equipment. Also, wash hands after decontamination carefully with antiseptic solution first and with soap afterwards. Do not open the instrument for decontamination inside. This is executed only by Service Technician.



Information

- To ensure decontamination of the instrument outer surfaces, clean the instrument surface at the end of the daily work. This has to be executed in the following three situations;
 - Regularly, at the end of a daily work,
 - Immediately, during contamination with potentially infectious material, and
 - In advance of repair or maintenance by the field technical service representative.
- Wipe off the instrument surfaces using a cloth soaked with a suitable decontamination solution. Please use one-way cloths, e.g. made of paper or cellulose. The cloth may be moistened in a way only that no wetness may reach the inside of the instrument.
- The indicated residence time of the decontamination solution shall be observed.
- If required, you may afterwards remove normal contaminations with commercial neutral detergent, in case these could not be removed by the decontaminant.
- As a last step the instrument shall be dried with a dry one-way cloth.

2.9 Operators



Caution!

- The instrument must only be used by properly trained personnel.
- In the event that a malfunction of the instrument occurs, take the measures indicated in the Instructions for Use. Further resolution should be referred to your Sysmex technical representative.

2.10 Computer viruses



Warning!

It has been verified that the instrument you have purchased is free of computer viruses. Antivirus software has been preinstalled in the instrument; however, before using an external memory device such as a USB memory stick, always verify that the device is free of viruses.


2.11 Use of other software

Warning!

- Do not install any software other than the software that is preinstalled on the instrument. Never run other software on the instrument.
- Note that we bear no liability whatsoever for any malfunctions arising from the use of other software.

2.12 Markings on the instrument

Front and side views (XN-530)

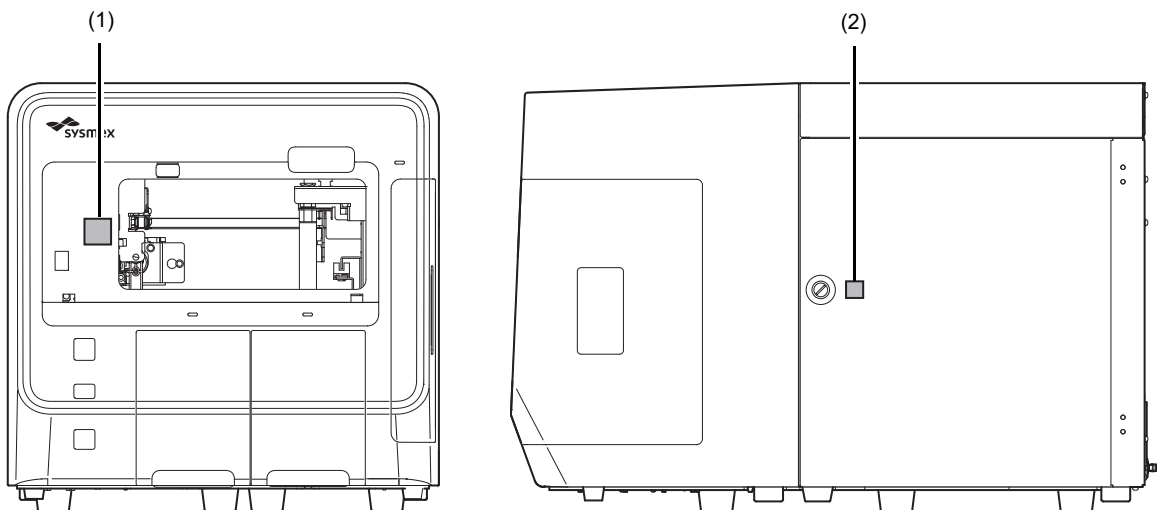

(1) Surfaces



Risk of infection


Treat all parts and surfaces of the instrument as posing a risk of infection.

(2) Right view

Warning!

Never insert your hand when the power of the analyzer is turned ON. There is a risk of injury.

Interior view (XN-530)

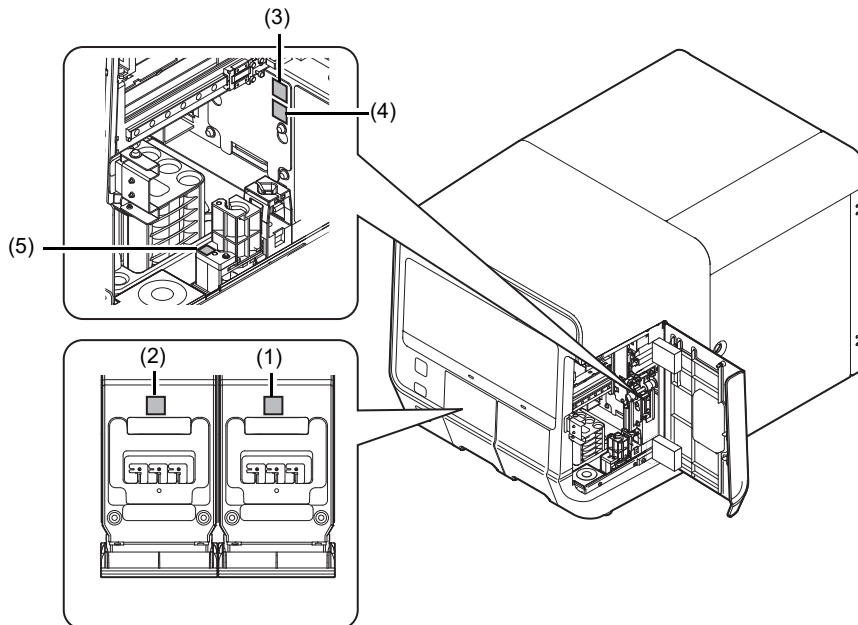

(1) Sampler adapter holder (right)



Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

(2) Sampler adapter holder (left)



Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

(3) Sampler adapter holder (interior)



Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

(4) Sampler adapter holder (interior)



Warning!

Never insert your hand when the power of the analyzer is turned ON. There is a risk of injury.


- (5) Sample tube holder



Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

Front, interior, and side views (XN-430)

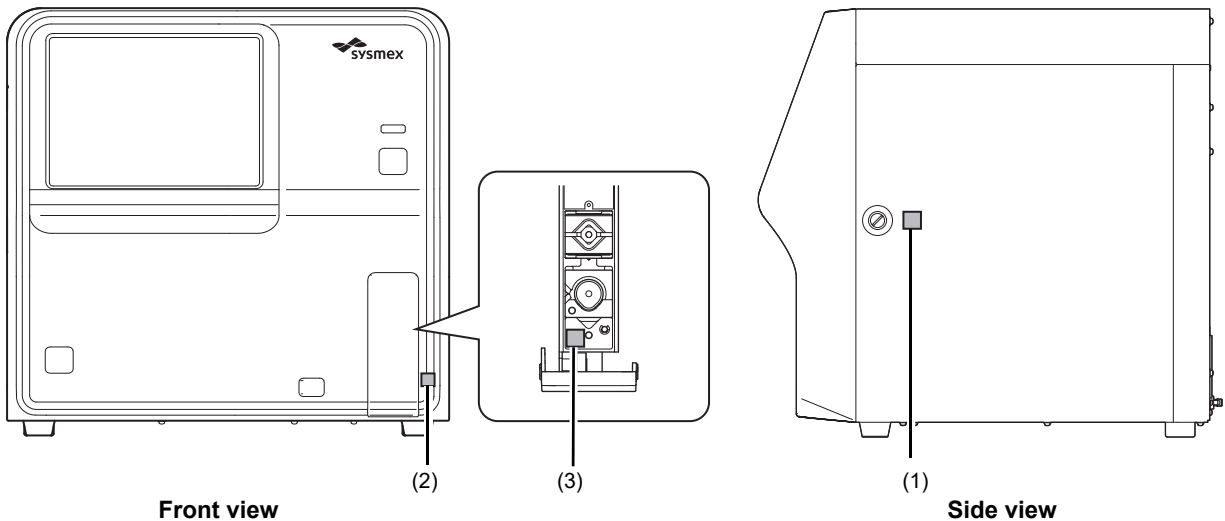

- (1) Right view



Warning!

Never insert your hand when the power of the analyzer is turned ON. There is a risk of injury.

- (2) Side of sample tube holder



Caution!

Never insert your hand. There is a risk of injury.


- (3) Sample tube holder




Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

Front and side views (XN-330)

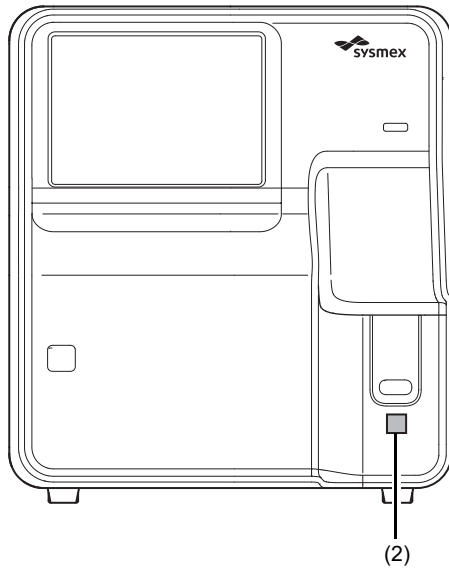

Front view

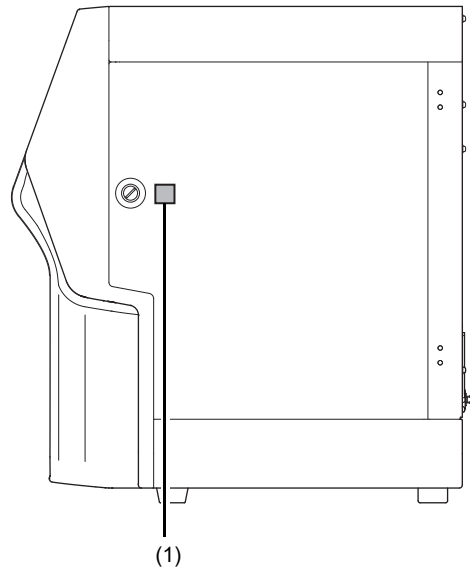

Side view

(1) Right view



Warning!


Never insert your hand when the power of the analyzer is turned ON. There is a risk of injury.

(2) Surfaces



Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

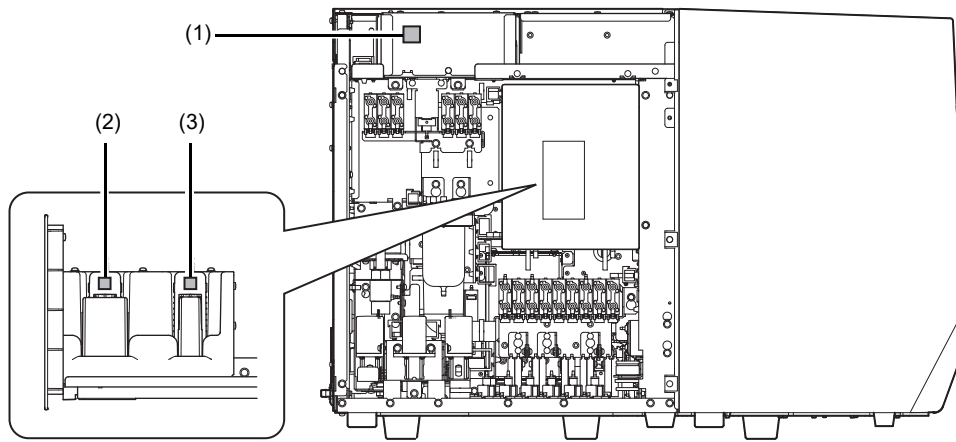Left interior (Common)**Example: XN-530**

- (1) Semiconductor laser unit

Warning!

The analyzers have a built-in semiconductor laser unit. To avoid the risk of eye injury, the laser is covered by a protective shielded box cover to prevent access by other than service technicians.

- (2) Fluorocell WDF dye cover

Warning!


Do not touch the nozzle.
There is a risk of injury.

- (3) Unused Fluorocell dye cover

Warning!

Do not touch the nozzle.
There is a risk of injury.

Right interior and top interior (Common)

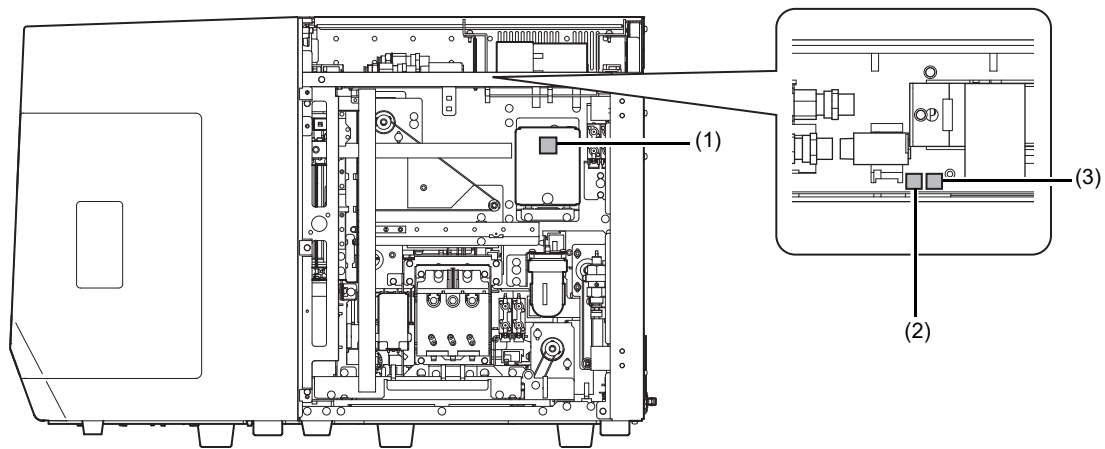

Example: XN-530

- (1) RBC detector cover



Warning!

To avoid electrical shock, unplug the power cable before servicing. An electrical shock could occur.

- (2) Air pump unit (top)



Warning!

To avoid electrical shock, unplug the power cable before servicing. An electrical shock could occur.


- (3) Air pump unit (top)



Caution, Hot!

The surface of the air pump is hot. Do not touch. There is a risk of burn injury.

Rear view (Common)

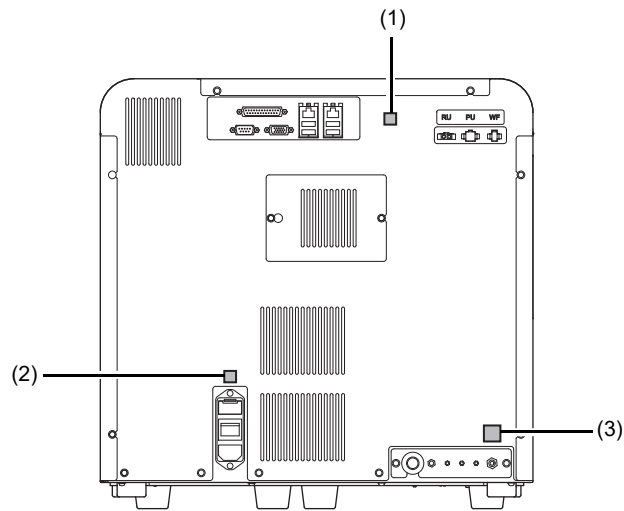

Example: XN-530

- (1) Interface connector

**Caution!**

Failure to observe this warning may result in instrument damage due to electrostatic discharge from your body.

- (2) Periphery of main power supply

**Warning!**


- To avoid electrical shock, unplug the power cable before servicing. An electrical shock could occur.
- Replace only with fuses of the specified type and current rating.

- (3) Waste fluid outlet nipple

**Risk of infection**

Treat all parts and surfaces of the instrument as posing a risk of infection.

Pneumatic unit (Option)

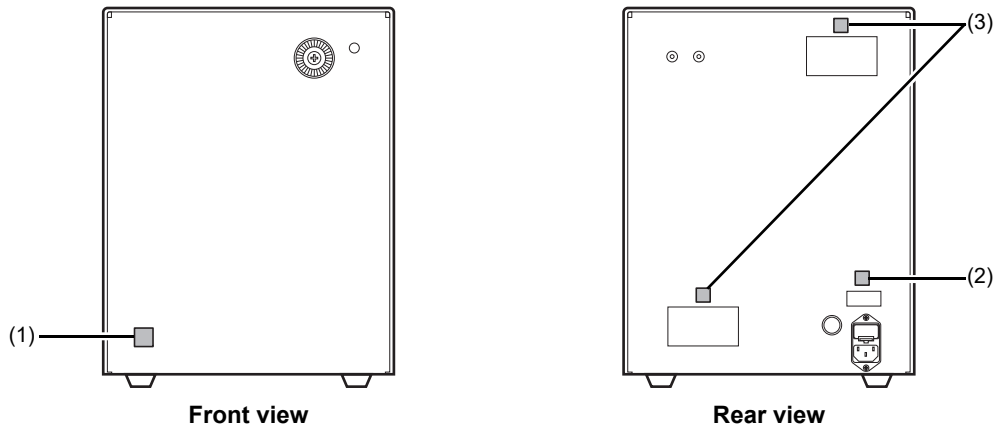

(1) Pneumatic unit



Risk of infection

Treat all parts and surfaces of the instrument as posing a risk of infection.

(2) Power connector



Warning!

- To avoid electrical shock, unplug the power cable before servicing. An electrical shock could occur.
- Use only a fuse of the specified type and rating. Doing so could cause a smoke emission and a fire.

(3) Exhaust vent



Caution!


Do not obstruct the exhaust vent on the back of the pneumatic unit.

Chapter 3 Part Names and Functions

This chapter explains an external view and overview of the instrument.

3.1 Analyzer

Front view (XN-530)

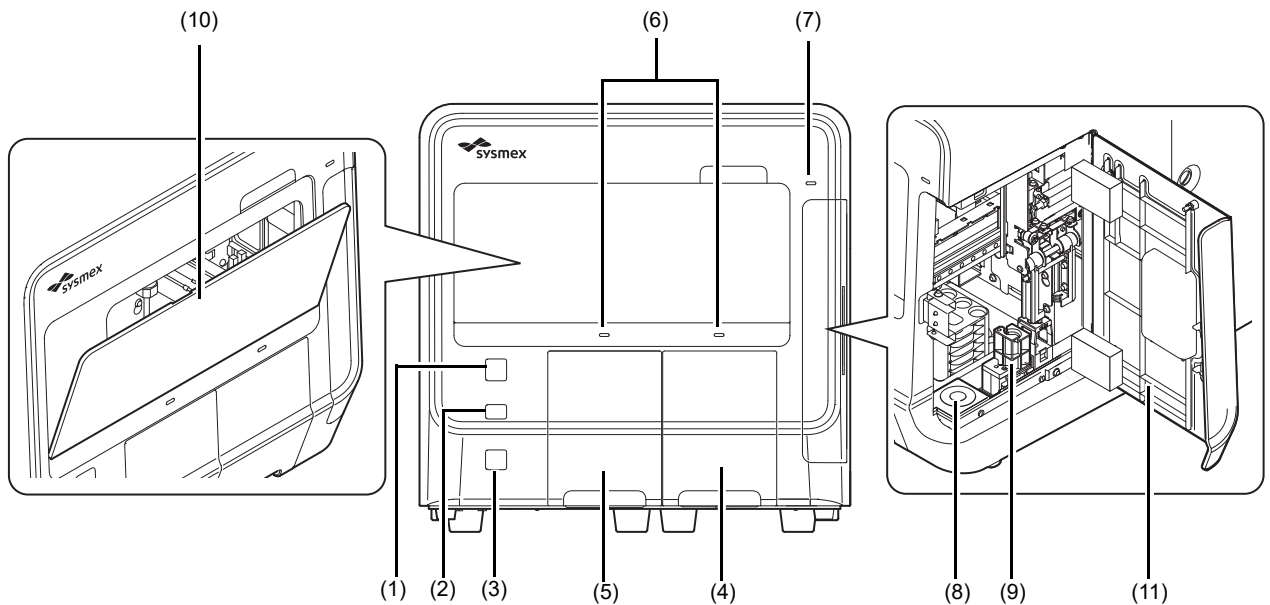

(1) Sampler start/stop switch

Press to start sampler analysis. Press to stop sampler analysis while sampler analysis is in progress.

(2) Mode switch

Press to switch between manual analysis mode and sampler analysis mode. Press while sampler analysis is in progress to change to manual analysis mode after analysis of the current sample is completed.

(3) Power switch

Turn the instrument power ON.

For procedures on turning OFF the instrument power, see "Basic Operation".

(►Basic Operation, "Chapter 1: 1.3 Shutdown")

(4) Sampler adapter holder (right)

Use to load sample tubes for sampler analysis mode.

(5) Sampler adapter holder (left)

Use to load sample tubes for sampler analysis mode.

(6) Sampler adapter status indicator LED

Indicates the status of the sampler adapter holder (right) / (left).

Not lit	All sample tubes in the sampler adapter have been analyzed, or there is no sampler adapter in the sampler adapter holder. The sampler adapter holder can be opened.
Green	Sampler adapter received state The sampler adapter holder can be opened.
Flashing green	Analysis in progress The sampler adapter holder cannot be opened. Wait until analysis is finished and then open the sampler adapter holder.
Red	Error occurring The sampler adapter holder can be opened.
Flashing red	Error occurring The sampler adapter holder cannot be opened. Wait until the sampler adapter status indicator LED lights solid red and then open the sampler adapter holder. For details on errors, see "Troubleshooting". (►Troubleshooting, "Chapter 1: 1.1 Error message list (in alphabetical order)")

(7) Manual analysis status indicator LED

Indicates the status of manual analysis.

Not lit	Sampler analysis mode
Green	Manual analysis is possible.
Flashing green	Aspirating a sample (during manual analysis).
Red	Error occurring

(8) Start switch

Press to start manual analysis.

(9) Sample tube holder


Use to load sample tubes for manual analysis mode.

(10) Sampler cover (front)

The cover can be removed for maintenance. The cover is not secured at the bottom. Take care not to drop the cover when removing it.

(11) Sampler cover (manual unit)

Open to load sample tubes for manual analysis mode.

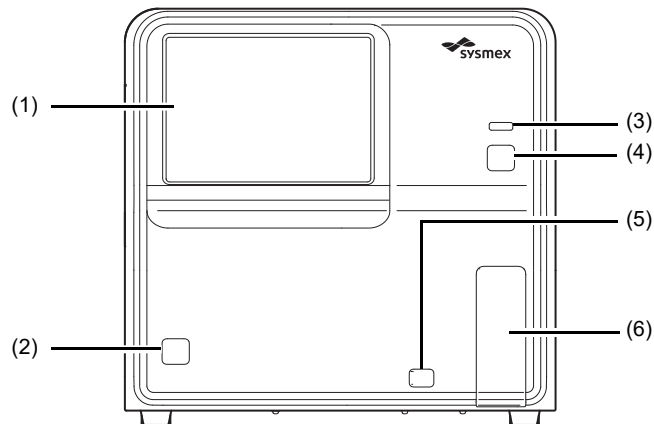Front view (XN-430)**(1) Touchscreen**

Use to operate the instrument and configure settings. The instrument status and analysis results can also be checked.

(2) Power switch

Turn the instrument power ON.

For procedures on turning OFF the instrument power, see "Basic Operation".

(►Basic Operation, "Chapter 1: 1.3 Shutdown")

(3) Analysis status indicator LED

Indicates the status of the analysis.

Green	Analysis is possible.
--------------	-----------------------

Flashing green	Aspirating a sample.
-----------------------	----------------------

Red	Error occurring
------------	-----------------

(4) Start switch


Press to start analysis.

(5) Sample tube holder open/close switch

Press to open and close the sample tube holder.

(6) Sample tube holder

Open to load sample tubes.

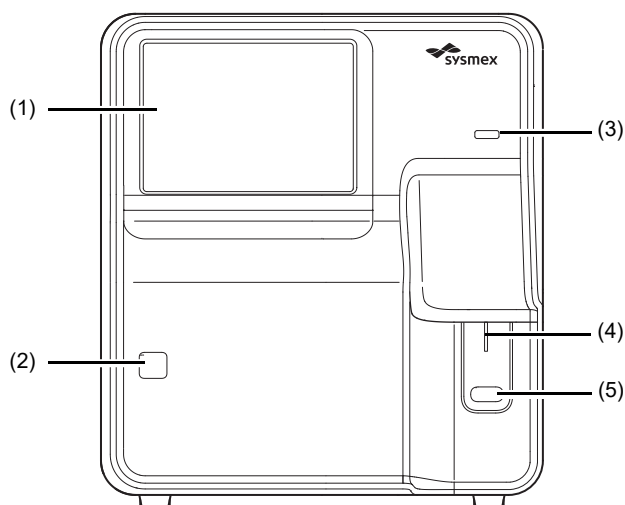Front view (XN-330)**(1) Touchscreen**

Use to operate the instrument and configure settings. The instrument status and analysis results can also be checked.

(2) Power switch

Turn the instrument power ON.

For procedures on turning OFF the instrument power, see "Basic Operation".

(►Basic Operation, "Chapter 1: 1.3 Shutdown")

(3) Analysis status indicator LED

Indicates the status of the analysis.


Green	Analysis is possible.
Flashing green	Aspirating a sample.
Red	Error occurring

(4) Aspiration pipette


Aspirates a sample.

(5) Start switch

Press to start analysis.

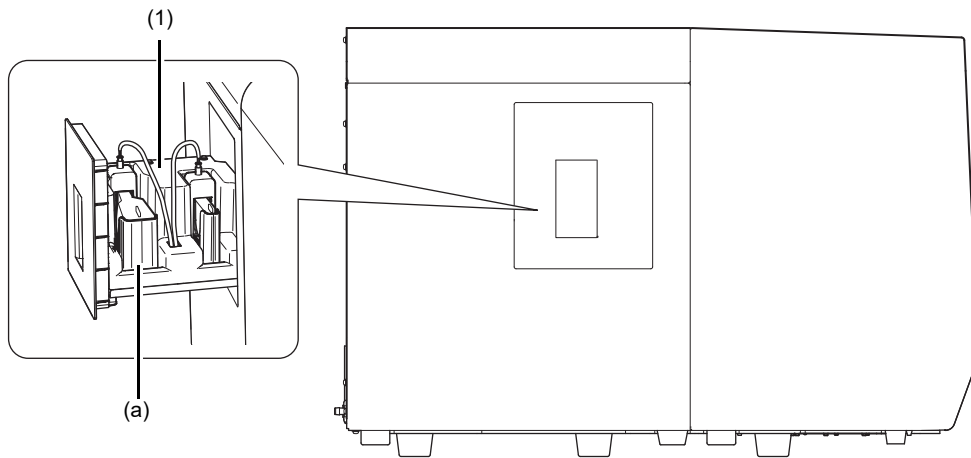Left view (Common)**Example: XN-530****(1) Dye holder**

Holds the fluorescence reagent.

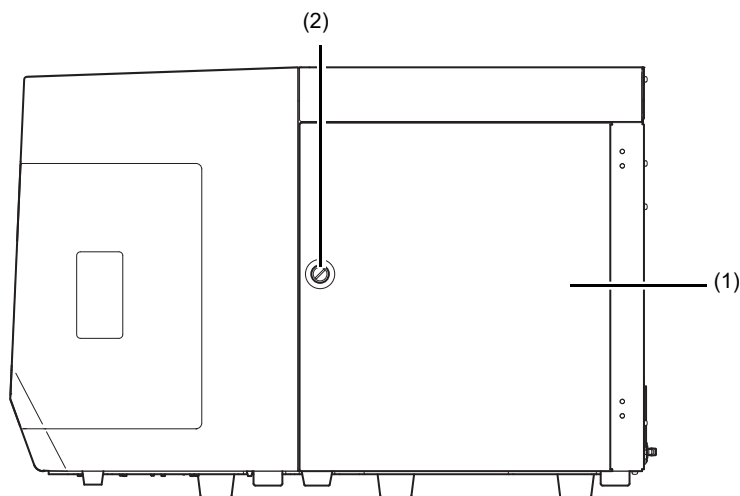
(a) Fluorocell WDF holder**Right view (Common)****Example: XN-530****(1) Right cover**

Open to inspect and perform maintenance on the inside of the analyzer.

(2) Lock

Lock for opening/closing of the right cover.


Right interior (Common)

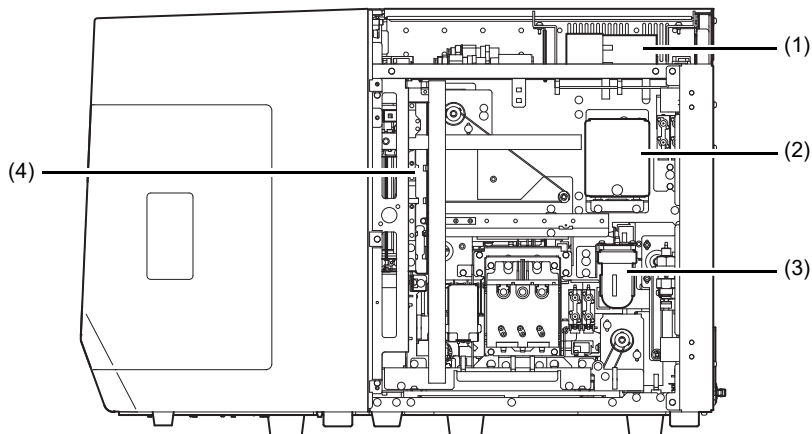

Example: XN-530

- (1) **Air pump unit**
Adjusts the air pressure that is supplied inside the instrument.
- (2) **RBC detector cover**
Contains an RBC detector.
- (3) **Pneumatic trap chamber**
Prevents reagent and other fluids from flowing into the air pump unit when an abnormality occurs in the instrument.
- (4) **Piercer (XN-530/XN-430)**
The piercer moves to the sample tube to aspirate the sample during analysis.

Rear view (Common)

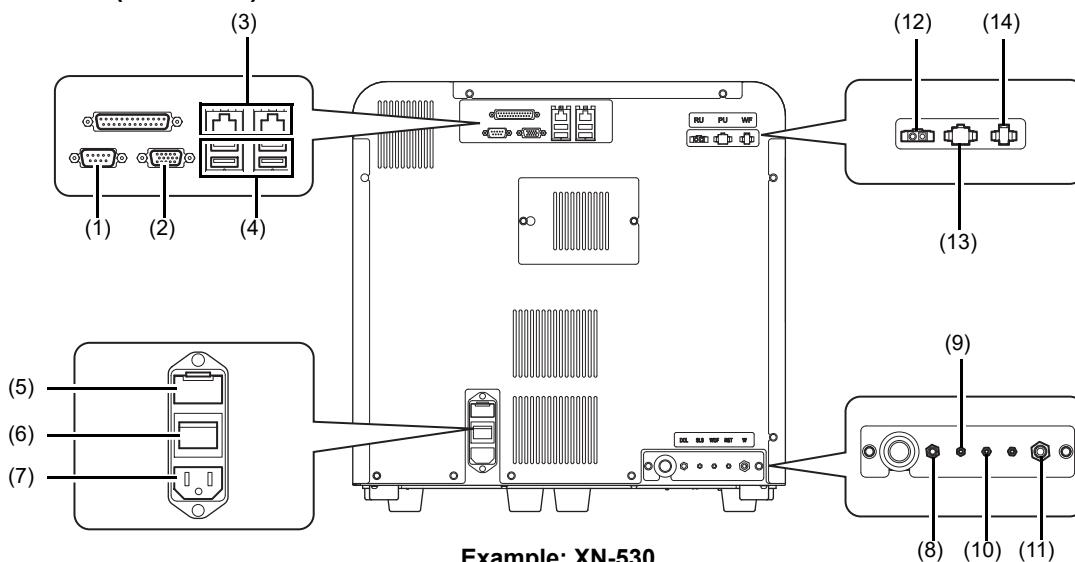

Example: XN-530

- (1) **RS-232C port**
Use to connect the instrument to a host computer.
- (2) **Monitor connection port (VGA)**
Use to connect to a monitor (XN-530 only).
- (3) **LAN port**
Use to connect to a host computer or SNCS (option).

(4) USB port

Use to connect to a monitor (XN-530 only), hand-held barcode reader (option), or printer (option). Insert a USB memory stick to back up and restore various types of files.

(5) Fuse holder

Use a 250 V, 10 A (time lag) fuse.

(6) Main power switch

Turn the main power of the instrument ON/OFF.

**Caution!**

Do not turn this switch ON/OFF repeatedly within a short time. This may overload the fuse and cause it to blow.

(7) AC power inlet

Supplies power using the provided power cable.

(8) DCL aspiration nipple

CELLPACK DCL or diluted CELLPACK DST is aspirated through this nipple.

(9) SLS aspiration nipple

SULFOLYSER is aspirated through this nipple. Connect to a SULFOLYSER container.

(10) WDF aspiration nipple

Lysercell WDF is aspirated through this nipple. Connect to a Lysercell WDF container.

(11) Waste fluid outlet nipple

Waste fluid is discharged through this nipple. Connect to a drain or waste container.

(12) RU-20 tank sensor connection port

Used for communication with the RU-20 tank sensor.

**Information**

If the RU-20 supply tank is not connected, connect an anti-static electricity connector to the RU-20 tank sensor connection port. Do not remove this connector.

(13) Port for pneumatic unit control

Output port for turning the pneumatic unit (option) ON/OFF. Connects the pneumatic unit control input connector of the pneumatic unit.


(14) Port for waste container full sensor

Connect to the waste container full sensor (option).

**Information**

If the waste container full sensor (option) is not connected, connect an anti-static electricity connector to the port for the waste container full sensor. Do not remove this connector.

3.2 Monitor (XN-530)

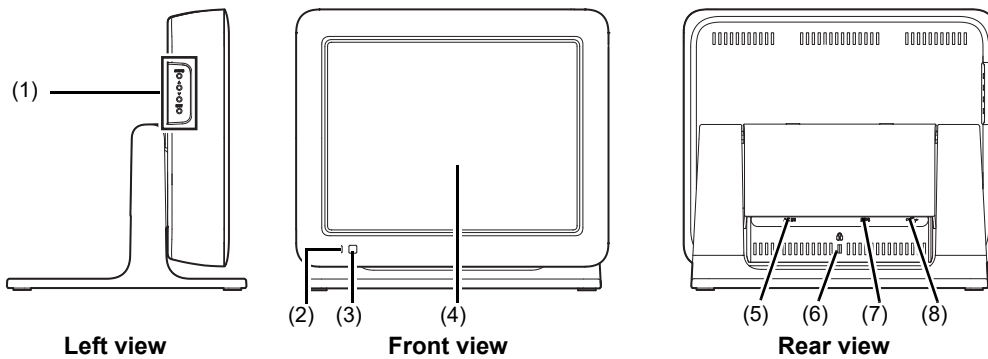

(1) OSD (on-screen display) operation buttons

Use to adjust the image quality.

(► Troubleshooting, "Chapter 2: 2.18 Adjusting the monitor image quality (XN-530)")

(2) Status LED

Indicates the status of the monitor.

Not lit	Power OFF
Green	Power ON, video signal input
Orange	Power ON, no video signal input*

* When there is no video signal input, [NO SIGNAL] appears and then the monitor enters the non-display state.

(3) Power switch

Turns the power of the monitor ON/OFF.

(4) Monitor (touchscreen)

Use to operate the instrument and configure settings. The instrument status and analysis results can also be checked.

(5) AC power inlet

Supplies power using the provided power cable.

(6) Security slot

Use to connect a commercially available anti-theft cable.

(7) RGB port

Connect the monitor to the analyzer. (Video signal)

(8) USB port

Connect the monitor to the analyzer. (Touchscreen signal)

Chapter 4 Installation

This chapter provides information regarding installation of the instrument.

4.1 Preparing for installation

The instrument is installed or moved by Sysmex service representatives. The following is a list of things to do beforehand to prepare for the installation or move.

- Secure ample space for installation, with safety considerations.
For the installation space, see the following.
(►P.39 "4.2.4 Installation space").
- Note the weight of this instrument. Make sure that the floor and/or the equipment on which the instrument is to be installed can withstand the weight.
- The power cable for this instrument is 2.0 m long. Use a nearby dedicated power outlet.
- Once this instrument is delivered, check the condition of its packaging as soon as possible.



Information

If the packaging has been damaged in any way, contact your Sysmex representative as soon as possible.

- Keep the instrument in its packaging in a dry place until it is time for installation. Store upright.

4.2 Installation

4.2.1 Cautions on installation

The instrument and associated equipment are installed by your Sysmex technical representative. In case relocation becomes necessary after installation, contact your Sysmex technical representative.

Problems resulting from moving of the instrument by anyone other than a Sysmex technical representative are not covered by the Warranty even within the warranty period.

4.2.2 Grounding

The safety plug of the power cord of the device must be connected to a properly grounded power outlet. An appropriate adaptor and plug type should be used in your region.

For details, please contact authorized local Sysmex representatives.



Warning!

- Be sure to ground this instrument.
Improper grounding may cause electrical shock.
- Never exceed socket capacity.
Failure to do so may cause a fire.



Caution!

Use the power cable that comes with the instrument. Do not use the power cable to supply power to any equipment other than the instrument.

4.2.3 Installation environment



- Use the instrument in an ambient temperature within the range of 15 to 35°C.
- Relative humidity should be within the range of 20 to 85%.
- If ambient temperature and relative humidity are not within the suggested range, air-condition the environment.

For other conditions, see Chapter 2. (► **P.16** "Chapter 2: 2.2 Installation")


4.2.4 Installation space

To allow sufficient space for maintenance, install the monitor unit on the left side of the analyzer. (XN-530 only)
Install the instrument with a clearance of at least 30 cm at the back.


Component	Width (mm)	Depth (mm)	Height (mm)	Weight (kg)
Analyzer (XN-530)	Approx. 450	Approx. 660	Approx. 450	Approx. 53
Monitor (XN-530)	Approx. 267	Approx. 205	Approx. 240	Approx. 3
Analyzer (XN-430)	Approx. 450	Approx. 460	Approx. 440	Approx. 35
Analyzer (XN-330)	Approx. 450	Approx. 460	Approx. 510	Approx. 35

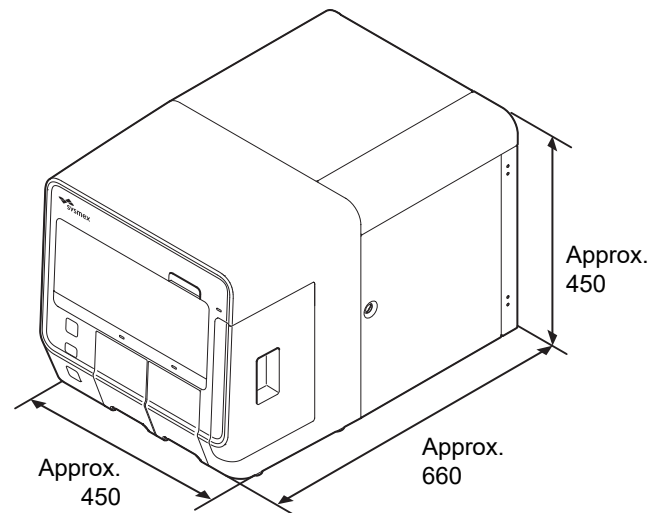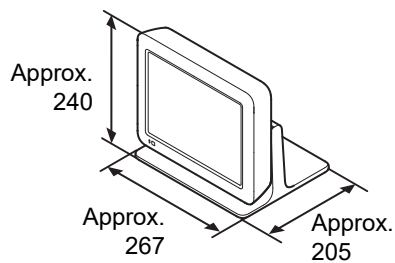

XN-530

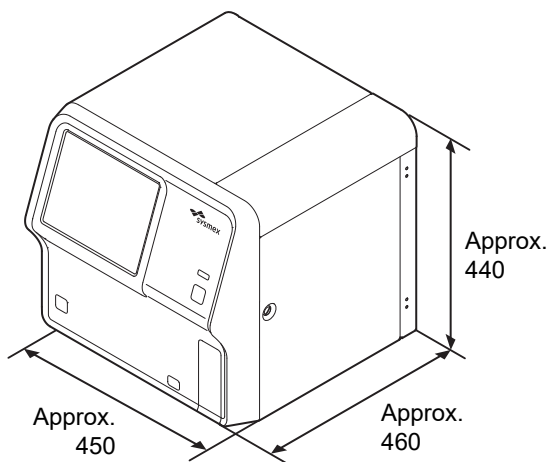

XN-430

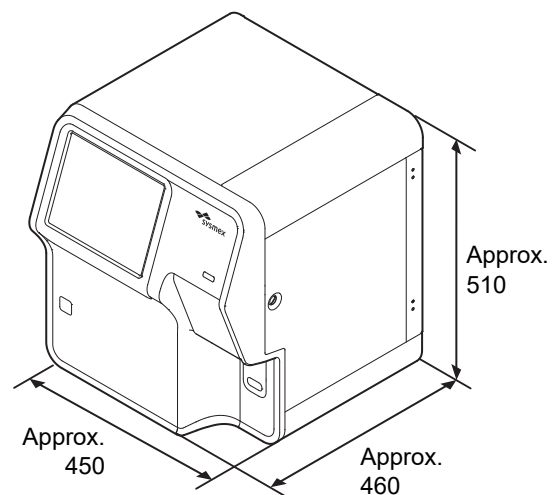

XN-330

Chapter 5 Instrument Specifications

This chapter explains technical information such as specifications and principles.

5.1 Specifications

Physical specifications (Analyzer)

Dimensions and weight	XN-530: Approx. 450 (W) x Approx. 660 (D) x Approx. 450 (H) mm, Approx. 53 kg XN-430: Approx. 450 (W) x Approx. 460 (D) x Approx. 440 (H) mm, Approx. 35 kg XN-330: Approx. 450 (W) x Approx. 460 (D) x Approx. 510 (H) mm, Approx. 35 kg
Electrical rating	Voltage: 100 to 240 V AC Frequency: 50/60 Hz Power consumption: XN-530: 250 VA XN-430/XN-330: 235 VA Protection type: Class I
Operating environment	Ambient temperature: 15 to 35°C (also applies to supplied reagents*) Relative humidity: 20 to 85% Atmospheric pressure: 70 to 106 kPa * Excluding CELLPACK DST.
Noise level	60 dB or less Excludes sound during clamping and release of sample tubes, and alarm sounds.
Storage conditions	Ambient temperature: -10 to 60°C Relative humidity: 10 to 95% (no condensation) Atmospheric pressure: 70 to 106 kPa
Laser class	Class I (IEC60825-1:2007)
Safety standards	IEC61010-1:2001, IEC61010-2-081:2001+A1, IEC61010-2-101:2002

Physical specifications (Monitor (XN-530))

Dimensions and weight	Approx. 267 (W) x Approx. 205 (D) x Approx. 240 (H) mm, Approx. 3 kg Monitor thickness: 52.5 mm
Electrical rating	Voltage: 100 to 240 V AC Frequency: 50/60 Hz Power consumption: 36 VA Protection type: Class I, limited to indoor use Over-voltage category: Category II
Storage conditions	Ambient temperature: -10 to 60°C Relative humidity: 10 to 95% (no condensation) Atmospheric pressure: 70 to 106 kPa
I/F specifications	Video signal I/F: Analog RGB signal (0.7 VP-P) Touch signal I/F: USB 2.0 compliant
I/F connectors	Video signal (analog RGB) input: Mini Dsub 15 pin (female) Touchscreen signal I/F (USB): USB 2.0 B connector AC power input: 3-prong plug
Supported resolutions	SVGA 800 x 3 (H) x 600 (V)
Screen size	26.4 cm (10.4 type) diagonal
Display colors	16,200,000 colors
Brightness	315 cd/m ² or more (typ 450 cd/m ²)
Contrast ratio (CR)	900:1
Angle of view	-60° to 80° (vertical), -80° to 80° (horizontal)
Backlight	LED
Touch detection method	4-wire analog resistive film type

Throughput

[Whole Blood] mode	When using the XN-530, the values below are for the case where the barcode reading function and Repeat/Rerun/Reflex function are not used. CBC: approx. 60 samples/hour CBC+DIFF: approx. 60 samples/hour
[Pre-Dilution] mode	CBC: approx. 60 samples/hour CBC+DIFF: approx. 60 samples/hour

Aspirated sample volume

[Whole Blood] mode	Sampler analysis: 25 µL Manual analysis: 25 µL Micro sample analysis: 25 µL Analysis using a micro collection tube: 25 µL Analysis using an RBT micro collection tube: 25 µL
[Pre-Dilution] mode	Micro sample analysis: 70 µL Analysis using a micro collection tube: 70 µL

Reportable parameters

For reportable parameters, see Chapter 1. (►P.10 "Chapter 1: 1.3 Reportable parameters")

Reportable range and display range

Parameters	Reportable range	Display range	Units
[Whole Blood] mode			
WBC	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
RBC	0.01 to 8.60	0.00 to 99.99	$\times 10^6/\mu\text{L}$
HGB	0.1 to 26.0	0.0 to 30.0	g/dL
HCT	0.1 to 75.0	0.0 to 100.0	%
MCV	NA ^{*1}	0.0 to 999.9	fL
MCH	NA ^{*1}	0.0 to 999.9	pg
MCHC	NA ^{*1}	0.0 to 999.9	g/dL
PLT	2 to 5000	0 to 9999	$\times 10^3/\mu\text{L}$
RDW-SD	NA ^{*2}	0.0 to 999.9	fL
RDW-CV	NA ^{*2}	0.0 to 999.9	%
MicroR	NA ^{*2}	0.0 to 100.0	%
MacroR	NA ^{*2}	0.0 to 100.0	%
PDW	NA ^{*2}	0.0 to 999.9	fL
MPV	NA ^{*1}	0.0 to 999.9	fL
P-LCR	NA ^{*2}	0.0 to 999.9	%
PCT	NA ^{*2}	0.00 to 99.99	%
NEUT#	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
LYMPH#	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
MONO#	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
EO#	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
BASO#	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
NEUT%	0.0 to 100.0	0.0 to 100.0	%
LYMPH%	0.0 to 100.0	0.0 to 100.0	%
MONO%	0.0 to 100.0	0.0 to 100.0	%
EO%	0.0 to 100.0	0.0 to 100.0	%
BASO%	0.0 to 100.0	0.0 to 100.0	%
IG#	0.03 to 440.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
IG%	0.0 to 100.0	0.0 to 100.0	%

*1 Not applicable, as this parameter is calculated from an equation.

*2 Not applicable, as this parameter is calculated using an equation from a distribution.

Reportable range and display range (continued)

Parameters	Reportable range	Display range	Units
[Pre-Dilution] mode			
WBC	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
RBC	0.01 to 8.60	0.00 to 99.99	$\times 10^6/\mu\text{L}$
HGB	0.2 to 26.0	0.0 to 30.0	g/dL
HCT	0.1 to 75.0	0.0 to 100.0	%
MCV	NA ^{*1}	0.0 to 999.9	fL
MCH	NA ^{*1}	0.0 to 999.9	pg
MCHC	NA ^{*1}	0.0 to 999.9	g/dL
PLT	5 to 1000	0 to 9999	$\times 10^3/\mu\text{L}$
RDW-SD	NA ^{*2}	0.0 to 999.9	fL
RDW-CV	NA ^{*2}	0.0 to 999.9	%
MicroR	NA ^{*2}	0.0 to 100.0	%
MacroR	NA ^{*2}	0.0 to 100.0	%
PDW	NA ^{*2}	0.0 to 999.9	fL
MPV	NA ^{*1}	0.0 to 999.9	fL
P-LCR	NA ^{*2}	0.0 to 999.9	%
PCT	NA ^{*2}	0.00 to 99.99	%
NEUT#	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
LYMPH#	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
MONO#	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
EO#	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
BASO#	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
NEUT%	0.0 to 100.0	0.0 to 100.0	%
LYMPH%	0.0 to 100.0	0.0 to 100.0	%
MONO%	0.0 to 100.0	0.0 to 100.0	%
EO%	0.0 to 100.0	0.0 to 100.0	%
BASO%	0.0 to 100.0	0.0 to 100.0	%
IG#	0.04 to 100.00	0.00 to 999.99	$\times 10^3/\mu\text{L}$
IG%	0.0 to 100.0	0.0 to 100.0	%

*1 Not applicable, as this parameter is calculated from an equation.

*2 Not applicable, as this parameter is calculated using an equation from a distribution.

Performance characteristics: Limit of blank, limit of detection, and limit of quantitation

The values below are from evaluation using a stabilized substance.

[Whole Blood] mode

Parameters	Limit of blank (LoB)	Limit of detection (LoD)	Limit of quantitation (LoQ)	Units
WBC ^{*1}	0.00	0.01	0.03	x 10 ³ /μL
RBC	0.00	0.00	0.01	x 10 ⁶ /μL
HGB	0.0	0.0	0.1	g/dL
PLT	0	1	2	x 10 ³ /μL
HCT	0.0	0.0	0.1	%
WBC ^{*2}	0.01	0.02	0.03	x 10 ³ /μL

*1 The white blood cell count measured from the WDF channel. (CBC+DIFF mode)

*2 The white blood cell count measured from the forward scattered light and the side scattered light of the WDF channel. (CBC mode)

[Pre-Dilution] mode

Parameters	Limit of blank (LoB)	Limit of detection (LoD)	Limit of quantitation (LoQ)	Units
WBC ^{*1}	0.00	0.01	0.03	x 10 ³ /μL
RBC	0.00	0.00	0.01	x 10 ⁶ /μL
HGB	0.0	0.1	0.2	g/dL
PLT	2	3	5	x 10 ³ /μL
HCT	0.0	0.1	0.1	%
WBC ^{*2}	0.02	0.03	0.04	x 10 ³ /μL

*1 The white blood cell count measured from the WDF channel. (CBC+DIFF mode)

*2 The white blood cell count measured from the forward scattered light and the side scattered light of the WDF channel. (CBC mode)

Linearity

[Whole Blood] mode	<p>Indicated as a logical value or a residual or residual rate with respect to the value measured on a standard instrument.</p> <p>WBC: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$)</p> <p>RBC: within $\pm 2\%$, or within $\pm 0.03 \times 10^6/\mu\text{L}$ (0.00 to $8.00 \times 10^6/\mu\text{L}$) within $\pm 4\%$, or within $\pm 0.06 \times 10^6/\mu\text{L}$ (8.01 to $8.60 \times 10^6/\mu\text{L}$)</p> <p>HGB: within $\pm 2\%$, or within ± 0.2 g/dL (0.0 to 26.0 g/dL)</p> <p>HCT: within $\pm 3\%$, or within ± 1.0 HCT (0.0 to 75.0%)</p> <p>MCV: NA^{*1}</p> <p>MCH: NA^{*1}</p> <p>MCHC: NA^{*1}</p> <p>PLT: within $\pm 5\%$, or within $\pm 10 \times 10^3/\mu\text{L}$ (0 to $1000 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (1001 to $5000 \times 10^3/\mu\text{L}$)</p> <p>RDW-SD: NA^{*2}</p> <p>RDW-CV: NA^{*2}</p> <p>MicroR: NA^{*2}</p> <p>MacroR: NA^{*2}</p> <p>PDW: NA^{*2}</p> <p>MPV: NA^{*1}</p> <p>P-LCR: NA^{*2}</p> <p>PCT: NA^{*2}</p> <p>NEUT#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$)</p> <p>LYMPH#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$)</p> <p>MONO#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$)</p> <p>EO#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$)</p> <p>BASO#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$)</p> <p>NEUT%: NA^{*3}</p> <p>LYMPH%: NA^{*3}</p> <p>MONO%: NA^{*3}</p> <p>EO%: NA^{*3}</p> <p>BASO%: NA^{*3}</p> <p>*1 Not applicable, as this parameter is calculated from an equation.</p> <p>*2 Not applicable, as this parameter is calculated using an equation from a distribution.</p> <p>*3 Not applicable, as this is a ratio.</p>
--------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Linearity (continued)

[Whole Blood] mode (continued)	IG#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) within $\pm 6\%$ (100.01 to $310.00 \times 10^3/\mu\text{L}$) within $\pm 11\%$ (310.01 to $440.00 \times 10^3/\mu\text{L}$) IG%: NA* * Not applicable, as this is a ratio.
[Pre-Dilution] mode	Indicated as a logical value or a residual or residual rate with respect to the value measured on a standard instrument. WBC: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) RBC: within $\pm 8\%$, or within $\pm 0.12 \times 10^6/\mu\text{L}$ (0.00 to $8.00 \times 10^6/\mu\text{L}$) HGB: within $\pm 5\%$, or within $\pm 0.5 \text{ g/dL}$ (0.0 to 26.0 g/dL) HCT: within $\pm 4\%$, or within $\pm 2.0 \text{ HCT}$ (0.0 to 75.0%) MCV: NA ^{*1} MCH: NA ^{*1} MCHC: NA ^{*1} PLT: within $\pm 10\%$, or within $\pm 20 \times 10^3/\mu\text{L}$ (0.0 to $1000 \times 10^3/\mu\text{L}$) RDW-SD: NA ^{*2} RDW-CV: NA ^{*2} MicroR: NA ^{*2} MacroR: NA ^{*2} PDW: NA ^{*2} MPV: NA ^{*1} P-LCR: NA ^{*2} PCT: NA ^{*2} NEUT#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) LYMPH#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) MONO#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) EO#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) BASO#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) NEUT%: NA ^{*3} LYMPH%: NA ^{*3} MONO%: NA ^{*3} EO%: NA ^{*3} BASO%: NA ^{*3} IG#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ (0.00 to $100.00 \times 10^3/\mu\text{L}$) IG%: NA ^{*3} *1 Not applicable, as this parameter is calculated from an equation. *2 Not applicable, as this parameter is calculated using an equation from a distribution. *3 Not applicable, as this is a ratio.

Precision (Repeatability)

[Whole Blood] mode	<p>Indicated as a coefficient of variation (95% reliability) of peripheral blood or control blood analyzed repeatedly 10 times or more.</p> <p>WBC: 3.0% or less ($4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>RBC: 1.5% or less ($4.00 \times 10^6/\mu\text{L}$ or more)</p> <p>HGB: 1.5% or less</p> <p>HCT: 1.5% or less</p> <p>MCV: 1.5% or less</p> <p>MCH: 2.0% or less</p> <p>MCHC: 2.0% or less</p> <p>PLT: 4.0% or less ($100 \times 10^3/\mu\text{L}$ or more)</p> <p>RDW-SD: 3.0% or less</p> <p>RDW-CV: 3.0% or less</p> <p>MicroR: 18.0% or less, or within ± 1.0 MicroR</p> <p>MacroR: 18.0% or less, or within ± 1.0 MacroR</p> <p>PDW: 10.0% or less</p> <p>MPV: 4.0% or less</p> <p>P-LCR: 18.0% or less</p> <p>PCT: 6.0% or less</p> <p>NEUT#: 8.0% or less ($1.20 \times 10^3/\mu\text{L}$ or more)</p> <p>LYMPH#: 8.0% or less ($0.60 \times 10^3/\mu\text{L}$ or more)</p> <p>MONO#: 20.0% or less ($0.20 \times 10^3/\mu\text{L}$ or more)</p> <p>EO#: 25.0% or less, or within $\pm 0.12 \times 10^3/\mu\text{L}$</p> <p>BASO#: 40.0% or less, or within $\pm 0.06 \times 10^3/\mu\text{L}$</p> <p>NEUT%: 8.0% or less (30.0 NEUT% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>LYMPH%: 8.0% or less (15.0 LYMPH% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>MONO%: 20.0% or less (5.0 MONO% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>EO%: 25.0% or less, or within ± 1.5 EO% (WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>BASO%: 40.0% or less, or within ± 1.0 BASO% (WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>IG#: 25.0% or less, or within $\pm 0.12 \times 10^3/\mu\text{L}$ (IG# $0.10 \times 10^3/\mu\text{L}$ or more)</p> <p>IG%: 25.0% or less, or within ± 1.5 IG% (2.0 IG% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p>
--------------------	---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Precision (Repeatability) (continued)

[Pre-Dilution] mode	<p>Indicated as a coefficient of variation (95% reliability) of a diluted sample of peripheral blood or control blood analyzed repeatedly 10 times or more.</p> <p>WBC: 5.0% or less ($4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>RBC: 4.5% or less ($4.00 \times 10^6/\mu\text{L}$ or more)</p> <p>HGB: 4.5% or less</p> <p>HCT: 4.5% or less</p> <p>MCV: 4.5% or less</p> <p>MCH: 4.5% or less</p> <p>MCHC: 6.0% or less</p> <p>PLT: 12.0% or less ($100 \times 10^3/\mu\text{L}$ or more)</p> <p>RDW-SD: 6.0% or less</p> <p>RDW-CV: 6.0% or less</p> <p>MicroR: 36.0% or less, or within ± 2.0 MicroR</p> <p>MacroR: 36.0% or less, or within ± 2.0 MacroR</p> <p>PDW: 20.0% or less</p> <p>MPV: 8.0% or less</p> <p>P-LCR: 36.0% or less</p> <p>PCT: 12.0% or less</p> <p>NEUT#: 16.0% or less ($1.20 \times 10^3/\mu\text{L}$ or more)</p> <p>LYMPH#: 16.0% or less ($0.60 \times 10^3/\mu\text{L}$ or more)</p> <p>MONO#: 40.0% or less ($0.20 \times 10^3/\mu\text{L}$ or more)</p> <p>EO#: 40.0% or less, or within $\pm 0.12 \times 10^3/\mu\text{L}$</p> <p>BASO#: 50.0% or less, or within $\pm 0.06 \times 10^3/\mu\text{L}$</p> <p>NEUT%: 16.0% or less (30.0 NEUT% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>LYMPH%: 16.0% or less (15.0 LYMPH% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>MONO%: 40.0% or less (5.0 MONO% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>EO%: 40.0% or less, or within ± 2.5 EO% (WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>BASO%: 50.0% or less, or within ± 1.5 BASO% (WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p> <p>IG#: 75.0% or less, or within $\pm 0.36 \times 10^3/\mu\text{L}$ (IG# $0.10 \times 10^3/\mu\text{L}$ or more)</p> <p>IG%: 75.0% or less, or within ± 4.5 IG% (2.0 IG% or more, WBC $4.00 \times 10^3/\mu\text{L}$ or more)</p>
---------------------	-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Precision (Reproducibility)

In the case of measuring the quality control material, the measurement values are within the limit values with respect to each target value.

Parameters	Level 1	Level 2	Level 3
RBC	within 5%	within 5%	within 5%
HGB	within 4%	within 4%	within 4%
HCT	within 10%	within 10%	within 10%
MCV	within 5%	within 5%	within 5%
MCH	within 9%	within 8%	within 8%
MCHC	within 15%	within 14%	within 14%
PLT	within 80%	within 15%	within 9%
RDW-SD	within 10%	within 10%	within 10%
RDW-CV	within 10%	within 10%	within 10%
PDW	within 80%	within 16%	within 12%
PCT	within 116%	within 30%	within 25%
WBC-C	within 10%	within 9%	within 9%
WBC-D	within 10%	within 8%	within 8%
NEUT#	within 20%	within 15%	within 15%
LYMPH#	within 40%	within 20%	within 20%
MONO#	within 80%	within 60%	within 50%
EO#	within 50%	within 50%	within 50%
BASO#	within 78%	within 78%	within 78%
NEUT%	within 20%	within 15%	within 15%
LYMPH%	within 40%	within 20%	within 20%
MONO%	within 80%	within 60%	within 50%
EO%	within 50%	within 50%	within 50%
BASO%	within 78%	within 78%	within 78%
IG#	within 30%	within 30%	within 25%
IG%	within 30%	within 30%	within 25%
MPV	within 9.0 fL	within 9%	within 7%
P-LCR	within 30.0 P-LCR%	within 50%	within 50%

Accuracy

[Whole Blood] mode	<p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood, and the value from analysis using a standard instrument.</p> <p>WBC: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ RBC: within $\pm 2\%$, or within $\pm 0.03 \times 10^6/\mu\text{L}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood and the value from analysis using a standard instrument or the international standard method (HGB standard analysis method of the cyanmethemoglobin method based on the ICSH (International Council for Standardization in Haematology)) advisory.</p> <p>HGB: within $\pm 2\%$, or within $\pm 0.2 \text{ g/dL}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood and the value from analysis using a standard instrument or the international standard method (standard analysis method based on the ICSH (International Council for Standardization in Haematology)) advisory.</p> <p>HCT: within $\pm 3\%$, or within $\pm 1.0 \text{ HCT}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>MCV: within $\pm 3\%$, or within $\pm 2.0 \text{ fL}$ MCH: NA^{*1} MCHC: NA^{*1}</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood and the value from analysis using a standard instrument or the international standard method (flow cytometry method based on the ICSH (International Council for Standardization in Haematology)) advisory.</p> <p>PLT: within $\pm 5\%$, or within $\pm 10 \times 10^3/\mu\text{L}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>RDW-SD: NA^{*2} RDW-CV: NA^{*2} MicroR: within $\pm 20\%$, or within $\pm 2.0 \text{ MicroR}$ MacroR: within $\pm 20\%$, or within $\pm 2.0 \text{ MacroR}$ PDW: NA^{*2} MPV: within $\pm 5\%$, or within $\pm 1.0 \text{ fL}$ (PLT $100 \times 10^3/\mu\text{L}$ or more) P-LCR: NA^{*2} PCT: within $\pm 5\%$, or within $\pm 0.03 \text{ PCT}$ (PLT $100 \times 10^3/\mu\text{L}$ or more)</p> <p>*1 Not applicable, as this parameter is calculated from an equation. *2 Not applicable, as this parameter is calculated using an equation from a distribution.</p>
--------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Accuracy (continued)

[Whole Blood] mode (continued)	<p>Indicated as a correlation coefficient with the reference data when 100 or more samples of peripheral blood are analyzed. The reference data is a standard instrument or standard analysis method of white blood cell 5 differentiation by flow cytometry.</p> <p>NEUT%: r = 0.90 or more LYMPH%: r = 0.90 or more MONO%: r = 0.75 or more EO%: r = 0.80 or more BASO%: r = 0.50 or more IG%: r = 0.80 or more</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>NEUT#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ LYMPH#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ MONO#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ EO#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ BASO#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ NEUT%: within ± 3.0 NEUT% LYMPH%: within ± 3.0 LYMPH% MONO%: within ± 2.0 MONO% EO%: within ± 1.0 EO% BASO%: within ± 1.0 BASO% IG#: within $\pm 3\%$, or within $\pm 0.30 \times 10^3/\mu\text{L}$ IG%: within ± 1.5 IG%</p>
-----------------------------------	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Accuracy (continued)

[Pre-Dilution] mode	<p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>WBC: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ RBC: within $\pm 8\%$, or within $\pm 0.12 \times 10^6/\mu\text{L}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument or the international standard method (HGB standard analysis method of the cyanmethemoglobin method based on the ICSH (International Council for Standardization in Haematology)) advisory.</p> <p>HGB: within $\pm 5\%$, or within $\pm 0.5 \text{ g/dL}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument or the international standard method (standard analysis method based on the ICSH (International Council for Standardization in Haematology)) advisory.</p> <p>HCT: within $\pm 4\%$, or within $\pm 2.0 \text{ HCT}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>MCV: within $\pm 4\%$, or within $\pm 3.0 \text{ fL}$ MCH: NA^{*1} MCHC: NA^{*1}</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument or the international standard method (flow cytometry method based on the ICSH (International Council for Standardization in Haematology)) advisory.</p> <p>PLT: within $\pm 10\%$, or within $\pm 20 \times 10^3/\mu\text{L}$</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>RDW-SD: NA^{*2} RDW-CV: NA^{*2} MicroR: within $\pm 40\%$, or within $\pm 3.0 \text{ MicroR}$ MacroR: within $\pm 40\%$, or within $\pm 3.0 \text{ MacroR}$ PDW: NA^{*2} MPV: within $\pm 7\%$, or within $\pm 1.5 \text{ fL}$ (PLT $100 \times 10^3/\mu\text{L}$ or more) P-LCR: NA^{*2} PCT: within $\pm 7\%$, or within $\pm 0.04 \text{ PCT}$ (PLT $100 \times 10^3/\mu\text{L}$ or more)</p> <p>*1 Not applicable, as this parameter is calculated from an equation. *2 Not applicable, as this parameter is calculated using an equation from a distribution.</p>
---------------------	---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Accuracy (continued)

[Pre-Dilution] mode (continued)	<p>Indicated as a correlation coefficient with the reference data when 100 or more diluted samples of peripheral blood are analyzed. The reference data is a standard instrument or standard analysis method of white blood cell 5 differentiation by flow cytometry.</p> <p>NEUT%: r = 0.70 or more LYMPH%: r = 0.70 or more MONO%: r = 0.60 or more EO%: r = 0.60 or more BASO%: r = 0.50 or more IG%: r = 0.80 or more</p> <p>Indicated as the average of the difference between the value from analysis of at least 100 diluted samples of peripheral blood and the value from analysis using a standard instrument.</p> <p>NEUT#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ LYMPH#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ MONO#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ EO#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ BASO#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$ NEUT%: within ± 3.0 NEUT% LYMPH%: within ± 3.0 LYMPH% MONO%: within ± 2.0 MONO% EO%: within ± 1.0 EO% BASO%: within ± 1.0 BASO% IG#: within $\pm 10\%$, or within $\pm 0.40 \times 10^3/\mu\text{L}$</p>
------------------------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Carryover

<p>[Whole Blood] mode / [Pre-Dilution] mode</p>	<p>Carryover is assessed by testing high levels of a parameter from peripheral blood or control blood three times followed by a diluent with low levels of a parameter. High to Low Carryover is calculated as follows:</p> $\text{Carryover} = \left[\frac{(\text{1st Low} - \text{3rd Low})}{(\text{3rd High} - \text{3rd Low})} \right] \times 100$ <p>WBC: 1.0% or less RBC: 1.0% or less HGB: 1.0% or less HCT: 1.0% or less MCV: NA^{*1} MCH: NA^{*1} MCHC: NA^{*1} PLT: 1.0% or less RDW-SD: NA^{*2} RDW-CV: NA^{*2} MicroR: NA^{*2} MacroR: NA^{*2} PDW: NA^{*2} MPV: NA^{*2} P-LCR: NA^{*2} PCT: NA^{*2} NEUT#: 2.0% or less, or 0.05 x 10³/μL or less LYMPH#: 2.0% or less, or 0.05 x 10³/μL or less MONO#: 2.0% or less, or 0.03 x 10³/μL or less EO#: 2.0% or less, or 0.03 x 10³/μL or less BASO#: 2.0% or less, or 0.03 x 10³/μL or less NEUT%: NA^{*3} LYMPH%: NA^{*3} MONO%: NA^{*3} EO%: NA^{*3} BASO%: NA^{*3} IG#: 2.0% or less, or 0.05 x 10³/μL or less IG%: NA^{*3}</p> <p>*1 Not applicable, as this parameter is calculated from an equation. *2 Not applicable, as this parameter is calculated using an equation from a distribution. *3 Not applicable, as this is a ratio.</p>
-----------------------------------------------------	------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------



Note:

If a low level sample is analyzed after a high level sample, the analysis results may be affected by carryover within the range of the carryover rate indicated in the table.

Sample stability with time after blood collection

Parameter	Stability Range	Units	18 to 26°C	2 to 8°C
WBC	within $\pm 10.0\%$	$\times 10^3/\mu\text{L}$	72 hours	-
RBC	within $\pm 5.0\%$	$\times 10^6/\mu\text{L}$	72 hours	-
HGB	within $\pm 5.0\%$	g/dL	72 hours	-
HCT	within $\pm 5.0\%$	%	8 hours	-
	within $\pm 8.0\%$	%	-	24 hours
	within $\pm 15.0\%$	%	24 hours	-
MCV	within $\pm 5.0\%$	fL	8 hours	-
	within $\pm 8.0\%$	fL	-	24 hours
	within $\pm 15.0\%$	fL	24 hours	-
PLT	within $\pm 10.0\%$, or within $\pm 30 \times 10^3/\mu\text{L}$	$\times 10^3/\mu\text{L}$	48 hours	-
MicroR	within $\pm 36.0\%$, or within ± 2.0 MicroR	%	8 hours	-
	within $\pm 36.0\%$, or within ± 2.0 MicroR	%	-	24 hours
MacroR	within $\pm 36.0\%$, or within ± 2.0 MacroR	%	8 hours	-
	within $\pm 36.0\%$, or within ± 2.0 MacroR	%	-	24 hours
NEUT%	within ± 8.0 NEUT%	%	48 hours	-
LYMPH%	within ± 7.0 LYMPH%	%	48 hours	-
MONO%	within ± 4.0 MONO%	%	48 hours	-
EO%	within ± 3.0 EO%	%	48 hours	-
BASO%	within ± 1.0 BASO%	%	-	12 hours
	within ± 1.0 BASO%	%	24 hours	-
IG%	within ± 2.0 IG%	%	24 hours	-

**Note:**

The sample used is stored at 18 to 26°C or in a refrigerator (2 to 8°C).
In the case of a refrigerated sample, the sample is returned to room temperature prior to analysis. Some samples may not fall within the above range, depending on the storage conditions.

Software specifications

Data storage capacity	Samples stored:	100,000 samples
	Patient information:	10,000 records
	Wards registered:	200 wards
	Doctor names registered:	200 names
	Analysis registration function:	2,000 records
	Calibration log:	20 records per analyzer
	QC files:	99 files per analyzer (300 plots per file)
	Reagent replacement log:	5,000 records
	Maintenance log:	5,000 records
Quality control (QC)	X-bar control (L-J control):	300 plots x 96 files
	X-barM control:	300 plots x 3 files

5.2 System limitations

5.2.1 Possible sample interferences

● WBC

If any of the following conditions are present, the system may erroneously report a low white blood cell count.

- Leukocyte aggregation

If any of the following conditions are present, the system may erroneously report a high white blood cell count.

- Platelet aggregation
- Poor hemolysis
- Erythroblast
- Erythrocyte aggregation (Cold agglutinin)
- Chyloemia
- Cryoprotein
- Cryoglobulin
- Fibrin
- Giant platelets

● RBC

If any of the following conditions are present, the system may erroneously report a low red blood cell count.

- Erythrocyte aggregation (Cold agglutinin)
- Microerythrocytes
- Fragmented red blood cells

If any of the following conditions are present, the system may erroneously report a high red blood cell count.

- Leukocytosis (> 100,000/ μ L)
- Giant platelets

● HGB

If any of the following conditions are present, the system may erroneously report a high hemoglobin value.

- Leukocytosis (> 100,000/ μ L)
- Lipemia
- Abnormal protein

● HCT

If any of the following conditions are present, the system may erroneously report a low hematocrit value.

- Erythrocyte aggregation (Cold agglutinin)
- Microerythrocytes
- Fragmented red blood cells

If any of the following conditions are present, the system may erroneously report a high hematocrit value.

- Leukocytosis ($> 100,000/\mu\text{L}$)
- Severe diabetes
- Uremia
- Spherocytosis

● PLT

If any of the following conditions are present, the system may erroneously report a low platelet count.

- Platelet aggregation
- Pseudothrombocytopenia
- Giant platelets

If any of the following conditions are present, the system may erroneously report a high platelet count.

- Microerythrocytes
- Fragmented red blood cells
- Fragmented leukocytes
- Cryoprotein
- Cryoglobulin

Interfering substances

Whole blood interference - EDTA-2K

Interfering substances studies for Bilirubin C, Bilirubin F, Hemolytic Hemoglobin, Lipemia (intralipid) and Chyle interferences were performed on the XN-L series.

A total of 6 whole blood EDTA-2K samples were collected from 3 donors each. All tubes were centrifuged and 150 μ L of plasma removed from each. Each interferent was diluted to (0%, 20%, 40%, 60%, 80%, and 100%) and then 150 μ L of each dilution was added to the centrifuged tubes (from a single donor). The tubes were mixed and measured 3 consecutive times for WBC, RBC, HGB, HCT, and PLT on the XN-L series.

Bilirubin C interference

There was no significant Bilirubin C interference up to a concentration of 42.2 mg/dL for WBC, RBC, HGB, HCT, and PLT parameters.

Bilirubin F interference

There was no significant Bilirubin F interference up to a concentration of 40.0 mg/dL for WBC, RBC, HGB, and HCT parameters, and up to a concentration of 8.0 mg/dL for PLT parameter.

Hemolysis interference

There was no significant hemolysis interference up to a concentration of 1018.0 mg/dL for WBC, RBC, HCT, and PLT parameters, and up to a concentration of 203.6 mg/dL for HGB parameter.

Intralipid interference

There was no significant intralipid interference up to a concentration of 2.00 g/dL for WBC, RBC, and HCT parameters, up to a concentration of 1.00 g/dL for PLT parameter, and up to a concentration of 0.20 g/dL for HGB parameter.

Chyle interference

There was no significant chyle interference up to a concentration of 2800 FTU for WBC^{*1}, RBC, HGB, and HCT parameters, and up to a concentration of 1680 FTU for PLT parameter. A significant chyle interference at a concentration of 560 FTU for WBC^{*2} parameter.

Allowable change rate:

The Allowable Change Rate is the allowable bias for each measurand. Bias outside the ranges listed below is considered an interference.

	WBC	RBC	HGB	HCT	PLT
Change rate	within \pm 10.9%	within \pm 3.2%	within \pm 2.8%	within \pm 2.8%	within \pm 9.1%

The concentration that showed no significant interference was judged by the change rate based on the criteria from the CLSI document H26-A2 under Biological variation (%CV) for all listed parameters.

*1 The white blood cell count calculated from the WDF channel (CBC+DIFF mode).

*2 The total white blood cell count calculated from the forward scattered light and the side scattered light of the WDF channel (CBC mode).


5.3 Supported sample tubes and sampler adapter

This section explains the sample tubes you can use with this instrument.

5.3.1 Supported sample tubes (XN-330)

● Regular sample tubes

Diameter (a)	φ11 to 15 mm
Length (b)	85 mm or less



5.3.2 Supported sample tubes (XN-530/XN-430)

● Regular sample tubes


Length including the cap (a)	70 to 85 mm
Diameter including the cap (b)	φ11 to 15 mm

With the exception of micro analysis, use the tube with the cap on.

Example: Sample tubes verified for correct operation

- VENOJECT II (Terumo)*
- Hemogard (BD)
- VACUETTE (Greiner)
- Monovette (SARSTEDT)

* Reusable caps cannot be used.



Caution!

When performing sampler analysis using VENOJECT II (Terumo), fold the film seal so that it does not protrude horizontally before placing in the rack. Otherwise, there is a risk that the seal will interfere with an adjacent sample tube and cause it to fall from the rack.



Note:


An adapter is needed when using a φ15 mm sample tube. For details, please contact your local Sysmex service representative.

- For XN-530 manual analysis / XN-430 analysis: XS adapter_ASSY (for φ15) 05357228
- For XN-530 sampler analysis: Adapter_ASSY No. 14 (15MM DIA) AR970823

● Micro collection tubes

Standard micro collection tube shapes are shown below.

Compatible dimensions vary depending on the shape of the micro collection tube. The following are guidelines. It will be necessary to check using the actual micro collection tube.

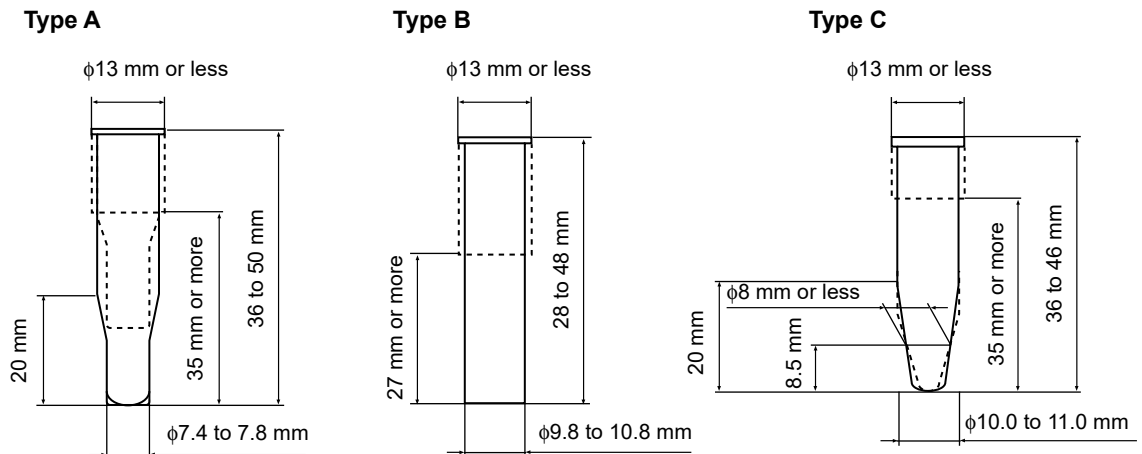

The cap is not included in the dimensions. Open the cap during analysis.

Example: Sample tubes verified for correct operation

- CAPIJECT CJ-NA (Terumo)
- The BD Microtainer Tube with BD Microgard Closure 365974 (BD)
- CAPIJECT II CJ-2DK (Terumo)*
- MiniCollect 450532 (Greiner)*

* The analyzer needs an adjustment if using the CAPIJECT II and MiniCollect. Please contact your Sysmex service representative.

● RBT micro collection tube (RBT: Raised Bottom Tube)

Micro collection tube that can be used for whole blood analysis on the XN-530 and XN-430. Allowable dimensions are the same as for regular sample tubes.

When using for sampler analysis, close the cap.

Example: Sample tubes verified for correct operation

- Microtainer MAP363706 (BD)




Caution!

Do not use a non-specified sample tube.

For information on using sample tubes not described here, contact your Sysmex service representative.


5.3.3 Supported sampler adapter

Regular sample tubes and RBT micro collection tubes can only be used with a Sysmex sampler adapter.

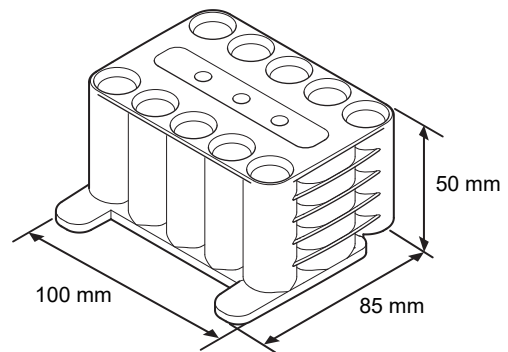

● Sample tube setup

Depending on the sample tube type, the metal fitting must be attached to the back of the sampler adapter.

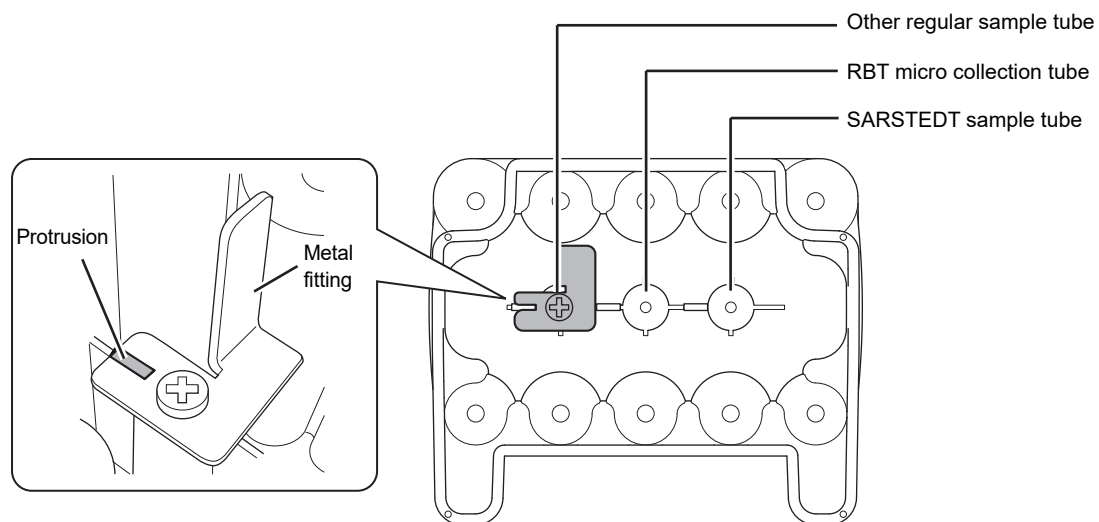

Example: Setup for other regular sample tubes


Caution!

- Use the sampler adapter with the metal fitting attached in the correct position for your sample tube type.
- Do not remove the attached metal fittings.
Reattaching metal fittings may cause screw loosening due to enlargement of screw holes.

5.4 Barcode labels (XN-530)

To correctly read a barcode using a sampler, the barcode label must be attached in the correct position.

Attach the barcode label to the sample tube so that the barcode is within the area shown on the right.

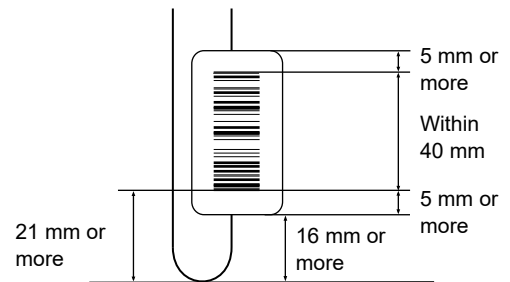

Caution!

When attaching barcode labels, pay attention to the points below. Incorrect attachment may cause barcode misreading and sample mix-ups.

- Attach the label so that the bars of the barcode are horizontal.
- Do not attach multiple labels.
- Do not allow the label to become wrinkled.
- Make sure that the label does not extend past the bottom of the sample tube.
- Make sure that the barcode label does not peel off the sample tube.
- Make sure that the labeled sample tubes can be inserted into and removed from the rack with ease.
- Do not write any text in the margins of a barcode label.

5.5 ID barcode specifications

This section explains the specifications of barcode labels that can be read by the hand-held barcode reader and the barcode reader on the XN-530 sampler.

5.5.1 Acceptable barcodes

The types of barcodes that can be used and check digit support are listed below.



Caution!

For the XN-530 only, use a check digit whenever possible when reading barcodes on sample tubes. There is a risk of incorrect reading of the barcode if a check digit is not used. To set a check digit, see "Basic Operation".

(►Basic Operation, "Chapter 7: 7.9.4 Barcode reader settings (XN-530)")

Sample numbers

Barcode types	Check digits	Number of digits
ITF	None	Max. 22 digits (sample No.)
	Modulus 10	Max. 21 digits (sample No.) + 1 digit (check digit) = Max. 22 digits
CODABAR/NW7	None	Max. 22 digits (sample No.)
	Modulus 11	Max. 22 digits (sample No.) + 1 digit (check digit) = Max. 23 digits
	Weighted modulus 11	
	Modulus 16	
CODE39	None	Max. 22 digits (sample No.)
	Modulus 43	Max. 22 digits (sample No.) + 1 digit (check digit) = Max. 23 digits
JAN/EAN/UPC	Modulus 10	12 digits (sample No.) + 1 digit (check digit) = 13 digits
ISBT128	Modulus 103	Max. 22 digits (sample No.) + 1 digit (check digit) = Max. 23 digits
CODE128	Modulus 103	Max. 22 digits (sample No.) + 1 digit (check digit) = Max. 23 digits



Information

When using CODE128, do not use the following codes.

Code	CODE A	CODE B
95	US	DEL
96	FNC 3	FNC 3
97	FNC 2	FNC 2
98	SHIFT	SHIFT
99	CODE C	CODE C
100	CODE B	FNC 4

Code	CODE A	CODE B
101	FNC 4	CODE A
102	FNC 1	FNC 1
103	START(CODE A)	
104	START(CODE B)	
105	START(CODE C)	

**Note:**

In CODE128, any one of the characters "A", "B", "C", "a", "b" or "c" can be used for the start/stop code.

Quality control (QC)

Barcode types	Check digits	Number of digits
CODE128	Modulus 103	3 digits (fixed character string [QC-]) + 8 digits (lot number) + 1 digit (check digit) = 12 digits

**Note:**

The CODE128 barcode for quality control is a special Sysmex code used for control blood.

5.5.2 Automatic assignment of sample numbers

A sample number is automatically assigned to samples when a barcode label read error occurs or when analysis begins while the analysis order was still being downloaded.

An automatically assigned sample number starts with a symbol that distinguishes it from other sample numbers.

Number starting with [ERR.]	Assigned when a barcode label read error occurs. A barcode label read error also occurs when a number includes characters that cannot be used. When a serial number is assigned and the limit number is exceeded, the number returns to [00....01].
Number starting with [QC]	Assigned to a QC sample with a lot number or to a QC file.
[BACKGROUNDCHECK]	Assigned to a background check sample.
Number starting with [PRE-CHK]	Assigned to a precision check sample.
Number starting with [CAL-CAL]	Assigned to samples calibrated by calibrator calibration.

**Information**

Sample numbers starting with [QC] whose lower 4 digits are one of the following numbers are assigned.

- "1401", "1402", "1403": XN-L CHECK

5.6 Functional descriptions

This device performs hematology analyses based on the Hydrodynamically focussed DC detection method, the flow cytometry method (using a semiconductor laser), and SLS-hemoglobin method.

5.6.1 Analysis principles


Hydrodynamically focussed DC detection method

The RBC detector counts RBC and PLT via the Hydrodynamically focussed DC detection method.

At the same time, the hematocrit (HCT) is calculated via the RBC pulse height detection method.

Inside the detector, the sample nozzle is positioned in front of the aperture and in line with the center. After diluted sample is forced from the sample nozzle into the conical chamber, it is surrounded by front sheath reagent and passes through the aperture center.

After passing through the aperture, the diluted sample is sent to the recovery tube. This prevents the blood cells in this area from drifting back, and prevents the generation of false platelet pulses. The Hydro Dynamic Focusing method improves blood cell count accuracy and repeatability. Because the blood cells pass through the aperture in a line, this method also prevents the generation of abnormal blood cell pulses.

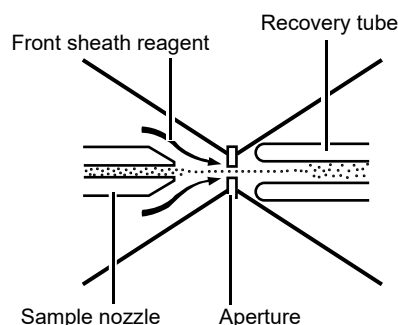


Flow cytometry method using semiconductor laser


Cytometry is used to analyze physiological and chemical characteristics of cells and other biological particles. Flow cytometry is a method used to analyze those cells and particles as they are passed through extremely small flow cells.

A blood sample is aspirated and measured, diluted to the specified ratio, and labeled. The sample is then fed into the flow cells by the sheath flow mechanism.

This mechanism improves cell count accuracy and repeatability. Since the blood cell particles pass in a line through the center of the flow cell, the generation of abnormal blood pulses is prevented and flow cell contamination is reduced.

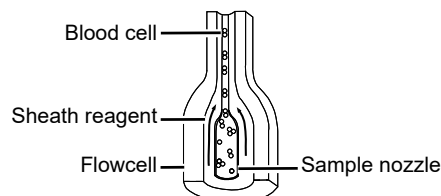

A semiconductor laser beam is directed onto the blood cells passing through the flow cell. The forward scattered light, side scattered light and side fluorescence are captured by the relevant photodiode. These lights are converted into electrical pulses, thus making it possible to obtain blood cell information.

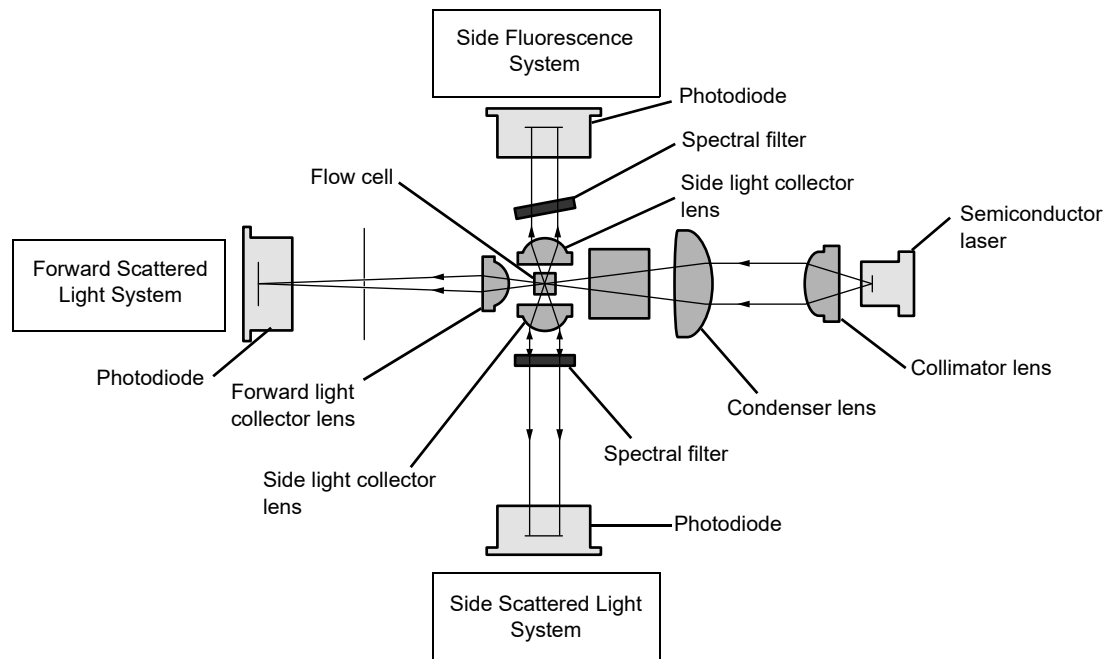

- Forward Scattered Light and Side Scattered Light

When obstacles pass through a light path, the light beam scatters from each obstacle in various directions. This phenomenon is called light scattering. By detecting the scattered light, it is possible to obtain information on cell size and material properties.

Likewise, when a laser beam is directed onto blood cell particles, light scattering occurs. The intensity of the scattered light depends on factors such as the particle diameter and viewing angle. This instrument detects forward scattered light, which provides information on blood cell size; and side scattered light, which provides information on the cell interior (such as the size of the nucleus).

- Side Fluorescence

When light is directed onto fluorescent material, such as labelled blood cells, light of longer wavelength than the original light is produced. The intensity of the fluorescence increases as the concentration of the marker becomes higher. By measuring the intensity of the fluorescence emitted, you can obtain information on the degree of blood cell labelling. Fluorescence is emitted in all directions. This instrument detects the fluorescence that is emitted sideways.

SLS-Hemoglobin Method

In the past, the mainstream methods for automatically measuring hemoglobin were the cyanmethemoglobin method and oxyhemoglobin method. These methods have both advantages and disadvantages when they are used with a large, fully automated instrument such as this instrument.

The cyanmethemoglobin method was recommended by the International Council for Standardization in Haematology (ICSH) in 1966 as an international standard method. However, because the hemoglobin conversion speed of this method is slow and multiple-sample processing is a requirement for automation, this method is not appropriate for automatic analysis. Moreover, the method uses cyanide compounds, which are poisonous, as reagents, and thus the liquid waste must be treated, making the method undesirable from an environmental perspective.

Currently this is not considered to be an appropriate analysis method for a large fully automatic instrument that discharges large amounts of liquid waste.

In contrast, the hemoglobin conversion speed of the oxyhemoglobin method is fast, as blood hemoglobin is instantly converted into oxyhemoglobin. In addition, it does not use poisonous substances such as cyanide, and thus is a suitable method for performing automatic analysis. The method cannot, however, convert methemoglobin into oxyhemoglobin, which is not a problem for normal human blood, but will result in values that are lower than the true values for samples that contain large amounts of methemoglobin, such as control blood samples.


The SLS-hemoglobin method is an analysis method that makes use of the advantages of the two aforementioned methods.

As with the oxyhemoglobin method, the hemoglobin conversion speed of the SLS-hemoglobin method is fast and the method does not use poisonous substances, making it a suitable method for automation.


Further, since methemoglobin can be analyzed, control samples such as control blood containing methemoglobin can also be accurately analyzed.

5.6.2 Hydraulic diagram

Whole blood mode

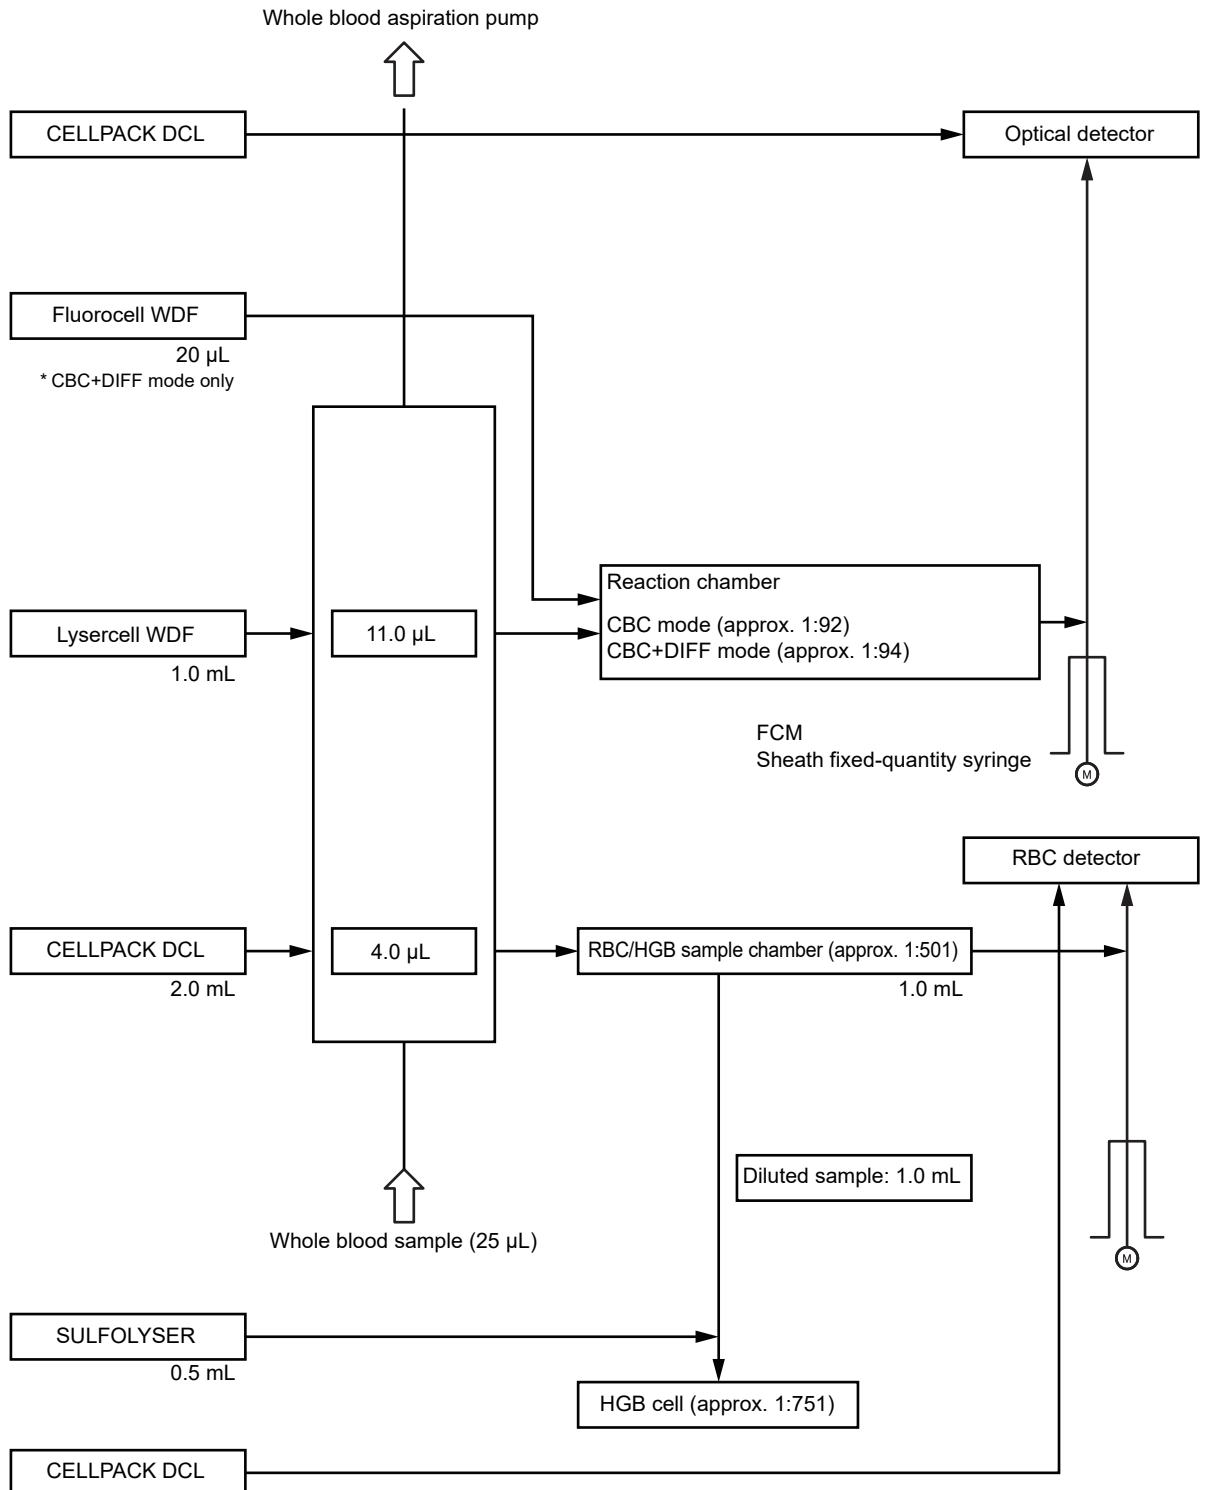

Pre-dilution mode

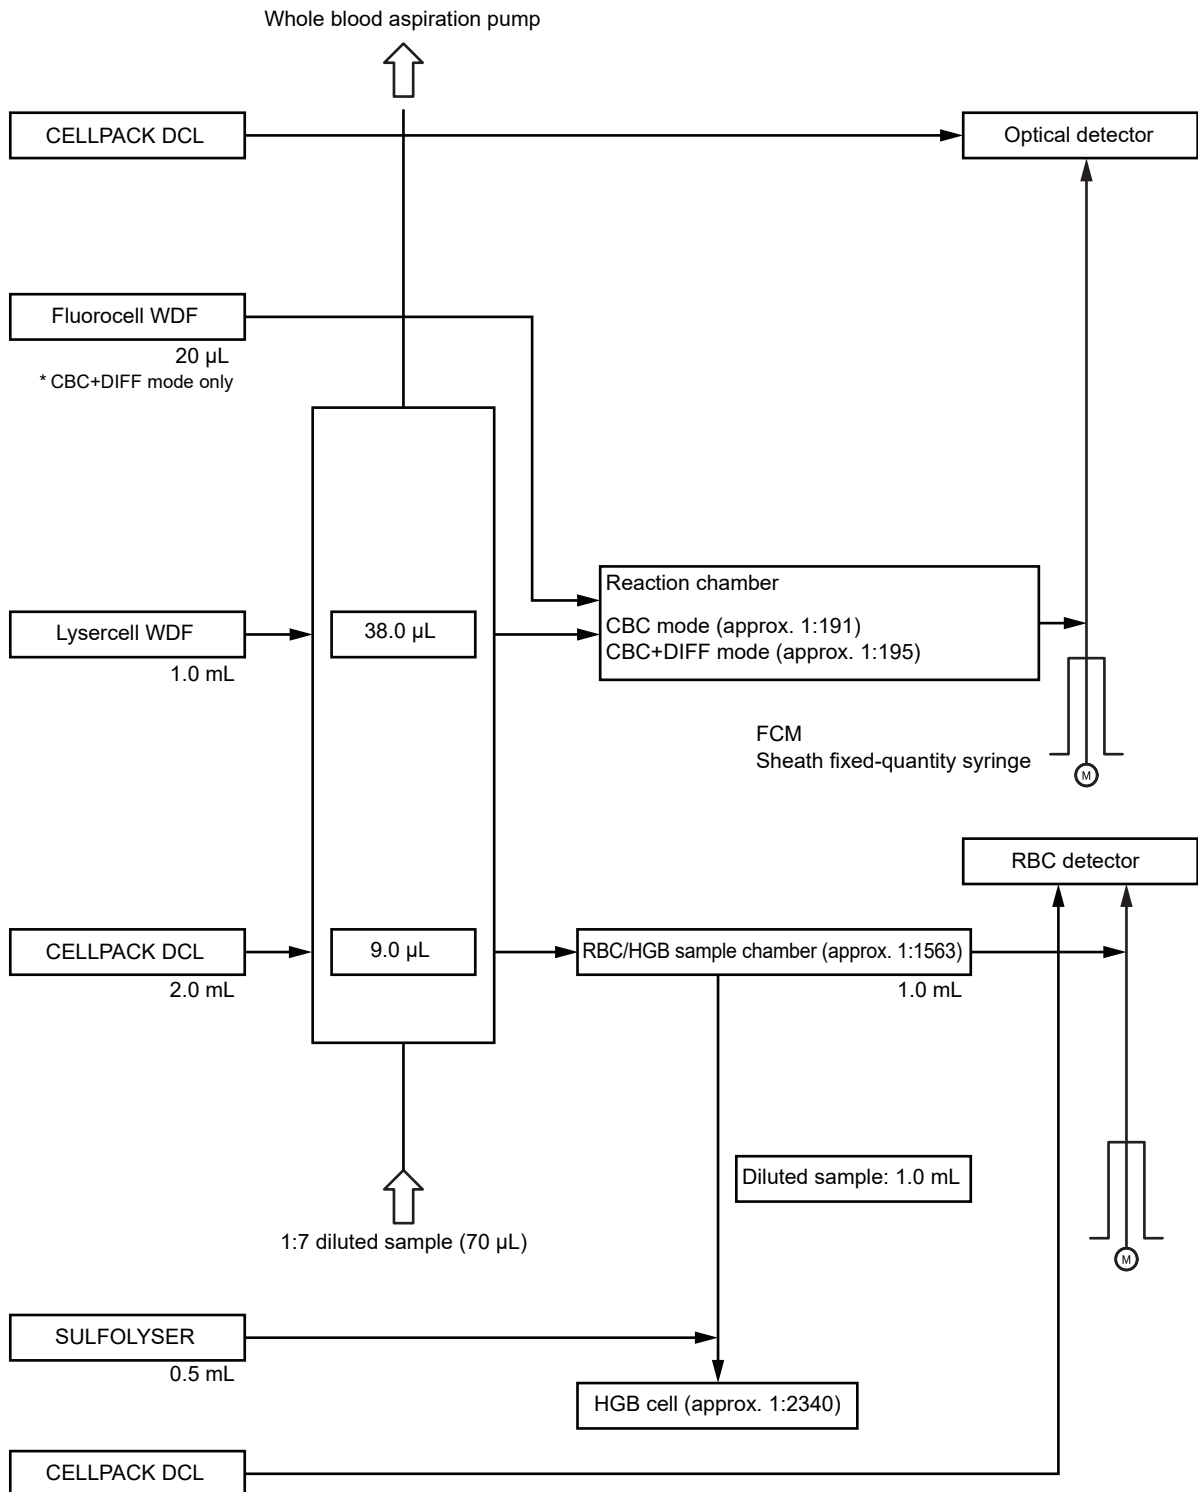

5.6.3 Reportable parameters and channels


WBC analysis

WDF channel

The WDF channel is a channel primarily for classifying white blood cells.

By flow cytometry method using a semiconductor laser, a 2-dimensional scattergram is drawn, with the X-axis representing the intensity of the side scattered light (SSC), and the Y-axis representing the intensity of the side fluorescence (SFL).

This scattergram displays clusters of lymphocytes, monocytes, eosinophils, neutrophils, basophils, and debris.

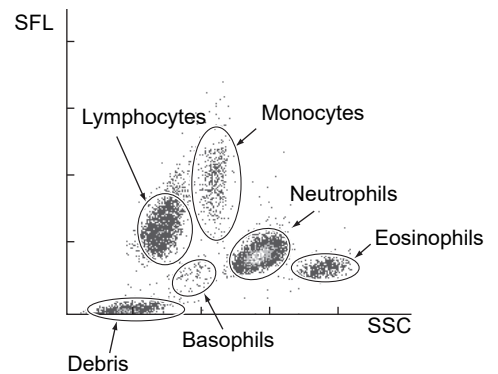

RBC/PLT analysis

RBC distribution

The RBC (red blood cell count) is calculated as a particle count between 2 discriminators (lower discriminator (LD) and upper discriminator (UD)), which are automatically set up in the ranges of 25 to 75 fL and 200 to 250 fL, respectively.


The particle size distribution is checked for abnormal relative frequencies at each discriminator level, abnormal distribution width, and the existence of more than 1 peak.

In this instrument, the RBC distribution width (RDW) is expressed in the following 2 ways.

● RDW-SD

With the peak height assumed to be 100%, the distribution width at the 20% frequency level is RDW-SD.


The unit used is fL (femtoliter) ($1 \text{ fL} = 10^{-15} \text{ L}$).

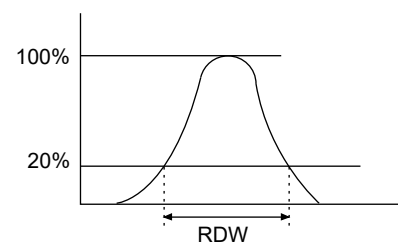

● RDW-CV

With points L1 and L2 found at a frequency of 68.26% of the total distribution area, RDW-CV is calculated from the following equation:

$$\text{RDW-CV (\%)} = \frac{L2-L1}{L2+L1} \times 100$$

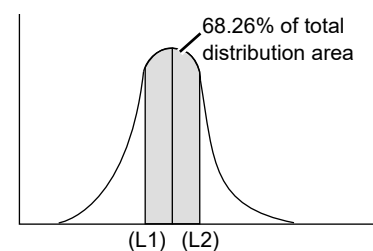

● **MCV (Mean cell volume)**

The MCV is calculated from the RBC and HCT, using the following equation:

$$\text{MCV (fL)} = \frac{\text{HCT (\%)}}{\text{RBC (x } 10^6/\mu\text{L)}} \times 10$$

● **MCH (Mean cell hemoglobin)**

The MCH is calculated from the RBC and HGB, using the following equation:

$$\text{MCH (pg)} = \frac{\text{HGB (g/dL)}}{\text{RBC (x } 10^6/\mu\text{L)}} \times 10$$

● **MCHC (Mean cell hemoglobin concentration)**

The MCHC is calculated from the HCT and HGB, using the following equation:

$$\text{MCHC (g/dL)} = \frac{\text{HGB (g/dL)}}{\text{HCT (\%)}} \times 100$$

PLT particle size distribution

The PLT (platelet count) is measured as a particle count between 2 discriminators (lower discriminator (LD) and upper discriminator (UD)), which are automatically set up in the ranges of 2 to 6 fL and 12 to 30 fL, respectively. PLT particle size distributions are checked for abnormalities, including abnormal relative frequencies at the lower discriminator, abnormal distribution widths, and the existence of more than 1 peak.


● **PDW (Platelet distribution width)**

With the peak height assumed to be 100%, the distribution width at the 20% frequency level is PDW.

The unit used is fL (femtoliter) (1 fL = 10⁻¹⁵ L).

● **P-LCR (Platelet-Large Cell Ratio)**

The P-LCR is the ratio of large platelets that are larger than the 12 fL discriminator. It is calculated as a ratio comparing the number of particles between the fixed discriminator (12 fL) and UD, to the number of particles between LD and UD.

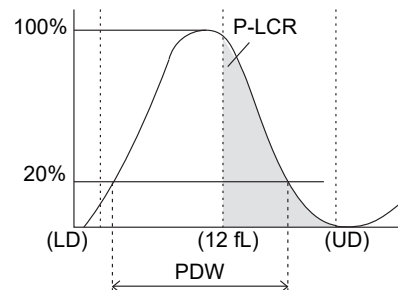

● **MPV (Mean Platelet Volume)**

The MPV is calculated from the following equation:

$$\text{MPV (fL)} = \frac{\text{PCT (\%)}}{\text{PLT (x } 10^4/\mu\text{L)}} \times 1000$$

PCT: PCT is called the platelet hematocrit or platelet volume ratio, and is weighted toward the PLT frequency.

Particle size distribution expression


The impression given by a particle size distribution can vary greatly, depending on the way in which it is expressed. The width of a particle size distribution requires particular attention because it can appear completely different, depending on the expression used for the distribution.

The instrument utilizes a conventional particle size distribution expression (normal expression) and a particle size distribution expression method that enables the user to obtain a large amount of information from the particle size distribution intuitively (normal cell size range expression).

● Normal expression

With the peak of the particle size distribution set as full scale (maximum height when the particle size distribution is displayed), this method of expression normalizes and expresses the distribution.

- Features:
 - Patterns of particle size distributions whose counts are different can be viewed on the same scale.
 - Widths of particle size distribution can be compared intuitively.
- Supported display area: RBC and PLT particle size distributions

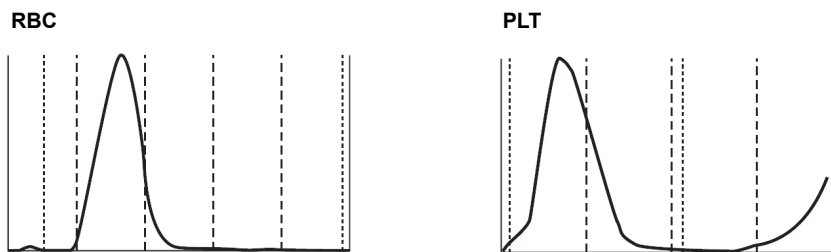


● Normal cell size range expression

This method of expression does not consider the peak of the particle size distribution as the full scale (maximum height when the particle size distribution is displayed). Instead, it normalizes the distribution, with the peak of the normal cell size range, which was calculated empirically, set as the full scale. At the same time, this method overlays the normal range of the particle size distribution.

If, however, the peak of the particle size distribution is higher than the peak of the normal cell size range, the expression is made with the distribution peak set as full scale. In this case, the normal cell size range is proportionally smaller than the height of the particle size distribution peak.

A normal cell size range can be obtained by superposing the particle size distributions of a large number of healthy people and then utilizing the region from the 10th percentile to the 90th percentile.

- Features:
 - The viewer can intuitively see the size of the particle count from the particle size distribution.
 - If the particle size distribution deviates from the normal range, the viewer knows instantly that the particle size distribution pattern is abnormal.
- Supported display area: RBC and PLT particle size distributions if settings are preset to normal range

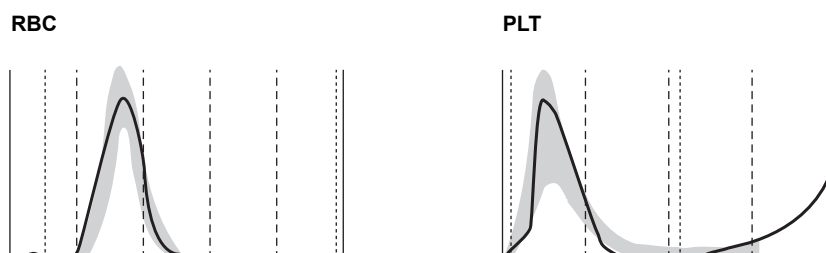

Chapter 6 Supplies, Accessories, and Options

This chapter describes the supplies, accessories, and options.

6.1 Supplies

Part number	Item name
26677681	Fuse 50T100H
05104711	Air pump set No. 1

6.2 Accessories

Part number	Item name	Quantity
AA835013	Intake Tube_ASSY No. 58 (For DCL 10 L)	1
CH037047	Intake Tube_ASSY No. 60 (For WDF 2 L bottle)	1
AE677153	Intake Tube_ASSY No. 62 (For SLS 500 mL bottle)	1
26571535	Power Cable TA-6P(A)+TA-5(A) H05VV-F	1 (XN-530: 2)
AF812533	Basic Operation	1
BA229091	Troubleshooting	1
AC044589	General Information	1
46235205	Brush (with cap)	1
46223818	Phillips head screwdriver	1
46223901	Flathead screwdriver	1
46231221	Opener No. 2 (Use to open CELLPACK DCL)	1
26677681	Fuse 50T100H	2
44253387	Tube 6x4	2 m
44253405	Tube 9x6	5 m
26644618	Tie wrap CV-100	10
BL006232	Tray No. 258 (Bottle stand)	1
BT850247	Cap No. 559 (Special opener for CELLCLEAN AUTO)	1
CP976529	Adapter No. 328 (Sampler adapter)	2 (XN-530 only)
BQ750561	Interrupter plate No. 395 (Metal fitting)	2 (XN-530 only)
66387687	Phillips head tapping screw bind M3×8	2 (XN-530 only)
AY707257	TM104-SYX01 (Monitor)	1 (XN-530 only)
04315817	Cable No. 3497 (Anti-static electricity connector for RU port)	1
96308015	Cable No. 2188 (Anti-static electricity connector for waste container full sensor)	1
BK659140	Label No. 1689	1 (XN-430/XN-330 only)

6.3 Options

Item name	Description
Graphic printer	Prints lists of analysis information and results.
List printer	Prints distributions, scattergrams and other analysis results, and hard copies of screens.
Waste container full sensor	Detects when the waste container is full.
Hand-held barcode reader	Scans a barcode on a sample tube and automatically inputs the sample number.
Pneumatic unit (PU-17)	Supplies positive/negative pressure to the instrument.

Chapter 7 Reagents

This chapter describes the reagents that are used with the instrument.

7.1 General information

All reagents used in this instrument are exclusively for use with Sysmex equipment. Do not use them for any other purpose. Please follow the warnings for handling and using each of the reagents correctly.

7.2 List of specified reagents

● Reagents

Product name	Storage temperature	Usage temperature	Shelf life after first opening	Composition
CELLPACK DCL	2 to 35°C	15 to 35°C	60 days	Sodium chloride 0.7% Tris buffer 0.2% EDTA-2K 0.02%
CELLPACK DST		15 to 30°C	60 days	Sodium chloride 15.7% Tris buffer 4.3% EDTA-2K 0.4%
SULFOLYSER	1 to 30°C	15 to 35°C	60 days	Sodium lauryl sulfate 1.7 g/L
Lysercell WDF	2 to 35°C		90 days	Organic quaternary ammonium salts 0.07% Nonionic surfactant 0.17%
Fluorocell WDF			90 days	Polymethine pigment 0.002% Methanol 3.0% Ethylene glycol 96.9%
CELLCLEAN AUTO	1 to 30°C		—	Sodium hypochlorite (Effective chlorine concentration 5.0%)

● Control blood and calibrator

Product name	Storage temperature	Usage temperature	Shelf life after first opening
XN-L CHECK	2 to 8°C	15 to 35°C	15 days
XN CAL			4 hours

7.3 CELLPACK DCL

Intended use

For in vitro diagnostic use only

CELLPACK DCL is a reagent for measuring the numbers and sizes of RBC and platelets by the Hydrodynamically focussed DC detection method. With the addition of the specified lyse reagent for hemoglobin concentration determination, it can also be used to analyze hemoglobin concentration. Also it can be used as a sheath fluid for FCM detector.

This reagent is to be used by connecting to an automatic hematology analyzer specified by Sysmex.

Warnings and precautions



Caution!

1. The reliability of the analysis values cannot be guaranteed if the reagent is used outside of the written intended use, or not according to the written directions for use.
2. When replacing the reagent, do not refill and use the same container.
3. Handle the reagent with care to prevent air bubbles from forming. If air bubbles form, analysis may not be performed normally.
4. Do not use expired reagents, as the reliability of the analysis values cannot be guaranteed.
5. If the reagent is removed after it has been connected (i.e. opened), it may become contaminated with bacteria and other particles, causing its performance to deteriorate. Therefore, reconnecting an open reagent is not recommended.
6. NEVER use this reagent on human body. Avoid contact with skin and eyes, and avoid ingestion. If it comes in contact with the skin, rinse skin thoroughly. If it gets in the eye, rinse with large amounts of water, and seek immediate medical attention. In the unlikely event that it was ingested, seek immediate medical attention.

Examination procedure

Use CELLPACK DCL at 15 - 35°C. If an analysis is performed at a temperature over 35°C or under 15°C, you may not be able to obtain accurate results. Connect the CELLPACK DCL container to the designated place on the instrument. For details, see "Troubleshooting". (►Troubleshooting "Chapter 2: 2.12 Replacing the reagent")

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store CELLPACK DCL at 2 - 35°C, away from direct sunlight. If the reagent has not been opened, it can be kept until the expiration date printed on the reagent container. For shelf life after opening (connecting to the instrument), refer to the expiration date printed on the reagent container or reagent specifications.

(►P.77 "7.2 List of specified reagents") Replace the reagent if it is showing signs of contamination or instability, such as cloudiness or discoloration. If frozen, thaw and mix thoroughly before use.

Disposal procedures

- 1 If crushing the container when disposing of fluid, make sure that any remaining fluid has been completely removed from the container before crushing.
- 2 Disposal procedures should meet requirements of applicable local regulations.

7.4 CELLPACK DST

Intended use

For in vitro diagnostic use only

CELLPACK DST is a reagent for measuring the numbers and sizes of RBC and platelets by the Hydrodynamically focussed DC detection method. With the addition of the specified lyse reagent for hemoglobin concentration determination, it can also be used to analyze hemoglobin concentration. Also it can be used as a sheath fluid for FCM detector.

This reagent is to be used by connecting to a reagent preparation device specified by Sysmex.

Warnings and precautions



Caution!

1. This reagent is a concentrated reagent. Use this reagent by connecting to a reagent preparation device specified by Sysmex.
2. The reliability of the analysis values cannot be guaranteed if the reagent is used outside of the written intended use, or not according to the written directions for use.
3. When replacing the reagent, do not refill and use the same container.
4. Handle the reagent with care to prevent air bubbles from forming. If air bubbles form, analysis may not be performed normally.
5. Do not use expired reagents, as the reliability of the analysis values cannot be guaranteed.
6. If the reagent is removed after it has been connected (i.e. opened), it may become contaminated with bacteria and other particles, causing its performance to deteriorate. Therefore, reconnecting an open reagent is not recommended.
7. NEVER use this reagent on human body. Avoid contact with skin and eyes, and avoid ingestion. If it comes in contact with the skin, rinse skin thoroughly. If it gets in the eye, rinse with large amounts of water, and seek immediate medical attention. In the unlikely event that it was ingested, seek immediate medical attention.
8. Before use, please read the Safety Data Sheet carefully.

Examination procedure

Use CELLPACK DST at 15 - 30°C. If an analysis is performed at a temperature over 30°C or under 15°C, you may not be able to obtain accurate results. Connect the CELLPACK DST container to the designated place on the reagent preparation device. For details, see "Troubleshooting".

(►Troubleshooting, "Chapter 2: 2.12 Replacing the reagent")

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store CELLPACK DST at 2 - 35°C, away from direct sunlight. If the reagent has not been opened, it can be kept until the expiration date printed on the reagent container. For shelf life after opening (connecting to the instrument), refer to the expiration date printed on the reagent container or reagent specifications.

(►P.77 "7.2 List of specified reagents") Replace the reagent if it is showing signs of contamination or instability, such as cloudiness or discoloration. Do not use a reagent that is suspected to have been frozen.

Disposal procedures

- 1 If crushing the container when disposing of fluid, make sure that any remaining fluid has been completely removed from the container before crushing.
- 2 Disposal procedures should meet requirements of applicable local regulations.

7.5 SULFOLYSER

Intended use

For in vitro diagnostic use only

SULFOLYSER is a reagent for the automated determination of hemoglobin concentration of blood with Sysmex automated hematology analyzers.

Warnings and precautions



Caution!

Avoid contact with skin and eyes. In case of skin contact, flush the area with water. In case of contact with eyes, rinse immediately with plenty of water and seek medical advice. If swallowed, seek medical advice immediately.

Examination procedure

1. Allow the container of SULFOLYSER to equilibrate to environmental temperature (15 - 35°C).
2. Loosen and remove the cap on the SULFOLYSER container.
3. Attach the Dispenser Kit to the SULFOLYSER container. Tighten the cap. Connect the SULFOLYSER line from the instrument to the Dispenser Kit.
4. Prime the SULFOLYSER through the hydraulic system of the instrument by cycling the instrument several times in the whole blood mode to fill all SULFOLYSER tubing with reagent and to remove air bubbles in the lines.

For details, see "Troubleshooting". (►Troubleshooting, "Chapter 2: 2.12 Replacing the reagent")

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store SULFOLYSER at 1 - 30°C, away from direct sunlight. If the reagent has not been opened, it can be kept until the expiration date printed on the reagent container. For shelf life after opening (connecting to the instrument), refer to the expiration date printed on the reagent container or reagent specifications. (►P.77 "7.2 List of specified reagents") Replace the reagent if it is showing signs of contamination or instability, such as cloudiness or discoloration.

Disposal procedures

- 1 If crushing the container when disposing of fluid, make sure that any remaining fluid has been completely removed from the container before crushing.
- 2 Disposal procedures should meet requirements of applicable local regulations.

7.6 Lysercell WDF

Intended use

For in vitro diagnostic use only

Lysercell WDF is a reagent used in combination with Fluorocell WDF. By hemolyzing red blood cells with Lysercell WDF and dyeing the white blood cell components with Fluorocell WDF, the counts and percentages of neutrophils, lymphocytes, monocytes, eosinophils, and basophils are analyzed. This reagent is to be used by connecting to an automated hematology analyzer specified by Sysmex.

Warnings and precautions



Caution!

1. The reliability of the analysis values cannot be guaranteed if the reagent is used outside of the written intended use, or not according to the written directions for use.
2. Handle the reagent with care to prevent air bubbles from forming. If air bubbles form, analysis may not be performed normally.
3. Do not use expired reagents, as the reliability of the analysis values cannot be guaranteed.
4. If the reagent is removed after it has been connected (i.e. opened), it may become contaminated with bacteria and other particles, causing its performance to deteriorate. Therefore, reconnecting an open reagent is not recommended.
5. NEVER use this reagent on human body. Avoid contact with skin and eyes, and avoid ingestion. If it comes in contact with the skin, rinse skin thoroughly. If it gets in the eye, rinse with large amounts of water, and seek immediate medical attention. In the unlikely event that it was ingested, seek immediate medical attention.

Examination procedure

Use Lysercell WDF at 15 - 35°C. If an analysis is performed at a temperature over 35°C or under 15°C, you may not be able to obtain accurate counts and percentages of neutrophils, lymphocytes, monocytes, eosinophils, and basophils. Connect the Lysercell WDF container to the designated place on the instrument. For details, see "Troubleshooting". (►Troubleshooting, "Chapter 2: 2.12 Replacing the reagent")

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store Lysercell WDF at 2 - 35°C, away from direct sunlight. If the reagent has not been opened, it can be kept until the expiration date printed on the reagent container. For shelf life after opening (connecting to the instrument), refer to the expiration date printed on the reagent container or reagent specifications.

(►P.77 "7.2 List of specified reagents") Replace the reagent if it is showing signs of contamination or instability, such as cloudiness or discoloration. Do not use a reagent that is suspected to have been frozen.

Disposal procedures

- 1 If crushing the container when disposing of fluid, make sure that any remaining fluid has been completely removed from the container before crushing.
- 2 Disposal procedures should meet requirements of applicable local regulations.

7.7 Fluorocell WDF

Intended use

For in vitro diagnostic use only

Fluorocell WDF is to be used to label the leukocytes in diluted and lysed blood samples for determination of the WBC differential with Sysmex automated hematology analyzers.

Warnings and precautions



Caution!

1. Wear gloves and a lab coat for protection. Avoid contact with skin and eyes.
2. In case of skin contact, rinse immediately with plenty of soap and water.
3. In case of contact with eyes, rinse immediately with water or normal saline, occasionally lifting upper and lower lids until no evidence of dye remains. Obtain medical attention.
4. If swallowed, seek medical advice immediately.
5. Do not breathe vapor. In case of accident or you feel unwell, seek medical advice immediately (show the label where possible).
6. Before use, please read the Safety Data Sheet carefully.

Examination procedure

1. Put a Fluorocell WDF cartridge in the prescribed position and then connect the Fluorocell WDF line.
2. Do not remove the IC tag until disposal. All the product information is managed by the IC tag on the label.
3. After setting, reset of the package is not recommended. Removing the reagent cartridge from the analyzer may cause deterioration of the reagent by contamination and opening in a sealing film.

For details, see "Troubleshooting". (►Troubleshooting, "Chapter 2: 2.12 Replacing the reagent")

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store Fluorocell WDF in a dark place at 2 - 35°C. If the reagent has not been opened, it can be kept until the expiration date printed on the package insert. For shelf life after opening (connecting to the instrument), refer to the expiration date printed on the package insert or reagent specifications. (►P.77 "7.2 List of specified reagents") Do not use a reagent that is suspected to have been frozen.

Disposal procedures

1. Tightly seal the spout of a cartridge before disposing to prevent residual reagent solution leaks. You may use tape to secure the spout.
2. Disposal procedures should meet requirements of applicable local regulations.

7.8 CELLCLEAN AUTO

Intended use

For in vitro diagnostic use only

CELLCLEAN AUTO is to be used as a strong alkaline detergent to remove SYSMEX lysing reagent, cellular residuals and blood proteins remaining in the hydraulics of XN series/XN-L series automated hematology analyzer and SP-10 automated hematology slide preparation unit.

Warnings and precautions



Warning!

Avoid contact with skin and eyes. In case of skin contact, flush the area with water. In case of contact with eyes, rinse immediately with plenty of water and seek medical advice.
Before use, please read the Safety Data Sheet carefully.

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store CELLCLEAN AUTO at 1 - 30°C, away from direct sunlight.

Do not use a reagent that is suspected to have been frozen.

Disposal procedures

- 1 After use, there will be a hole in the film that seals the top of the tube. Exercise caution, as residual fluid may leak from the hole.
- 2 Disposal procedures should meet requirements of applicable local regulations.

7.9 Control blood (XN-L CHECK)

Intended use

For in vitro diagnostic use only

XN-L CHECK is intended to be used as a control for complete blood cell count (CBC), white blood cell differential and reticulocyte parameters on Sysmex XN-L series instruments.

Warnings and precautions



Risk of infection

Always wear protective garments and gloves when using control blood. Also, wash your hands after completing the process.

The basic blood used in the control blood has tested negative for HBs antigen, HCV/HIV-1/HIV-2 antibodies, and serologic tests for syphilis. However, there are no tests that can completely rule out any infections. In addition, it has not been tested for other viruses. Therefore, handle the control blood with the same level of care you would use when handling other blood samples that may be infectious.



Caution!

1. Minimize the time that the product is left at room temperature.
Leaving the product at room temperature for a prolonged period of time will cause deterioration.
2. If suspected to have been frozen, the product cannot be used, as analysis results will be affected.

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store the control blood in a dark refrigerated place at 2 - 8°C.

If it has not been opened, the product can be kept until the expiration date printed on the vial label and outer box.

For shelf life after opening, refer to the package insert or reagent specifications. (►P.77 "7.2 List of specified reagents")

7.10 Calibrator (XN CAL)

Intended use

For in vitro diagnostic use only

Used for the calibration of the analyzer for WBC, RBC, HGB, HCT, and PLT.

Warnings and precautions



Risk of infection

Always wear protective garments and gloves when using calibrator. Also, wash your hands after completing the process.

The basic blood used in the calibrator has tested negative for HBs antigen, HCV/HIV-1/HIV-2 antibodies, and serologic tests for syphilis. However, there are no tests that can completely rule out any infections. In addition, it has not been tested for other viruses. Therefore, handle the control blood with the same level of care you would use when handling other blood samples that may be infectious.



Caution!

1. Minimize the time that the product is left at room temperature.
Leaving the product at room temperature for a prolonged period of time will cause deterioration.
2. If suspected to have been frozen, the product cannot be used, as analysis results will be affected.

Storage and shelf life of unopened product

Storage and shelf life after first opening

Store the calibrator in a dark refrigerated place at 2 - 8°C.

If it has not been opened, the product can be kept until the expiration date printed on the vial label and outer box.

For shelf life after opening, refer to the package insert or reagent specifications. (►P.77 "7.2 List of specified reagents")

Chapter 8 Service Data and Research Parameters

This chapter describes service data and research parameters.

8.1 Checking service data

Service data of samples within the [Sample Explorer] list can be reviewed by selecting the [Service] tab of the [Data Browser] screen*.

* Even when the data is masked in other confirmation screens, the values are displayed. When analysis is not executed on the channel for which the displayed item is measured, the data is not displayed.



Information

Data displayed on the [Service] tab is for the purpose of monitoring the status of the instrument. These data must not be used for diagnosis of patients.

Touch the [Service] tab in the [Data Browser] screen to display the following screen.

The screenshot shows the 'Data Browser' interface with the 'Service' tab selected. The top toolbar includes buttons for Menu, QC File, Explorer, Browser, Switch, Modify, Validate, Last 10, Output, Upper, Lower, and Delete. The main area displays the following data:

Sampling Data		Reference Data		Distribution	
RBC	PLT	R-MFV	L-RBC	RBC	
907	350	97.8 fL	0.00 10 ⁶ /uL	PLT	
969	382	P-MFV 10.4 fL	0.00 10 ⁶ /uL	PLT	
968	372	L-MCV 0.0 fL	236 10 ³ /uL		
963	383	S-MCV 0.0 fL			
955	408				
942	298				
941	366				
936	363				
974	389				
935	393				
477	208				
0	0				
0	0				
0	0				
0	0				
0	0				
0	0				
9039 (*8)	3614 (*1)				

Reference Data (continued):

RBC-LD	6	PLT-LD	1
RBC-MD			
RBC-UD	49	PLT-UD	29

HGB:

11.8 g/dL	11.79 g/dL	Sample	6226
7.3 mmol/L	7.32 mmol/L	Blank	5047

Distribution (continued):

RBC	
Clog	97
Bubble	0

[Data Browser] screen ([Service] tab)

The [Service] tab consists of 4 screens. To change the screen, touch the [Switch] button on the toolbar and change using the submenu that appears.

[RBC/PLT]	Displays the details of RBC/PLT data.
[WDF]	Displays the details of WDF data.
[HARDWARE]	Displays the details of HARDWARE data.
[ADJUSTMENT]	Displays the details of ADJUSTMENT data.

8.1.1 [RBC/PLT] service data

To display the information below, touch the [Switch] button - [RBC/PLT] on the toolbar.

[Sampling Data]	This sampling data is used to monitor the occurrence of sudden noise. If the difference between the maximum value and the minimum value constitutes a proportion of the total sampling value that exceeds the specified range, a sampling error will occur. <ul style="list-style-type: none"> • The particle count of the RBC/PLT channel measured at fixed intervals appears in the column below [RBC] and [PLT]. • The data of maximum of 32 measurements is displayed. • The total particle count appears at the bottom of the table. • The total count is normalized by a multiple of the value in the parentheses so that the total particle count falls into the range of 0 to 9999.
[Reference Data]	
[R-MFV]	Most frequent value for the red blood cell volume. (Units: fL)
[P-MFV]	Most frequent value for the platelet volume. (Units: fL)
[L-MCV]	MCV of the larger distribution of the 2 peak RBC distributions.
[S-MCV]	MCV of the smaller distribution of the 2 peak RBC distributions.
[L-RBC]	The red blood cell count of the larger distribution of the 2 peak RBC distributions.
[S-RBC]	The red blood cell count of the smaller distribution of the 2 peak RBC distributions.
[PLT-I]	The platelet count measured from the RBC/PLT channel (PLT distribution).
[Discr]	
[RBC-LD]	The position of the lower discriminator of the RBC distribution. (Numerical value from 0 to 49 with 49 full scale)
[RBC-MD]	The position of the discriminator that separates the 2 peak RBC distributions into a distribution with a smaller MCV and a distribution with a larger MCV. (Numerical value from 0 to 49 with 49 full scale)
[RBC-UD]	The position of the upper discriminator of the RBC distribution. (Numerical value from 0 to 49 with 49 full scale)
[PLT-LD]	The position of the lower discriminator of the PLT distribution. (Numerical value from 0 to 39 with 39 full scale)
[PLT-UD]	The position of the upper discriminator of the PLT distribution. (Numerical value from 0 to 39 with 39 full scale)
[HGB]	Hemoglobin values appear in 4 formats in the right column.
[Sample]	Optical density of the sample converted by A/D conversion.
[Blank]	Optical density of a blank sample converted by A/D conversion.
[Distribution]	
[RBC]	If the RBC distribution is abnormal, abnormal distribution information will be displayed.
[PLT]	If the PLT distribution is abnormal, abnormal distribution information will be displayed.
[RBC]	
[Clog]	Electronically detected numerical value indicating the amount of clogging in the RBC detector.
[Bubble]	Electronically detected numerical value indicating the amount of air bubbles in the RBC detector.

8.1.2 [WDF] service data

To display the information below, touch the [Switch] button - [WDF] on the toolbar.

[Sampling Data]	This sampling data is used to monitor the occurrence of sudden noise. If the difference between the maximum value and the minimum value constitutes a proportion of the total sampling value that exceeds the specified range, a sampling error will occur. <ul style="list-style-type: none"> • The particle count of the WDF channel measured at fixed intervals appears in the column below [WDF]. • The data of maximum of 16 measurements is displayed. • The total particle count appears at the bottom of the table. • The total count is normalized by a multiple of the value in the parentheses so that the total particle count falls into the range of 0 to 9999.
[Scattergram Sensitivity]	
[WDF-X]	The side scattered light intensity of the WBC area in the WDF scattergram.
[WDF-Y]	The fluorescence intensity of the WBC area in the WDF scattergram.
[NE-SSC]	The side scattered light intensity of the NEUT area in the WDF scattergram.
[NE-SFL]	The fluorescence intensity of the NEUT area in the WDF scattergram.
[WDF-WX]	The side scattered light distribution width index of the WBC area in the WDF scattergram.
[WDF-WY]	The fluorescence distribution width index of the WBC area in the WDF scattergram.
[LY-X]	The side scattered light intensity of the LYMPH area in the WDF scattergram.
[LY-Y]	The fluorescence intensity of the LYMPH area in the WDF scattergram.
[Reference Data]	
[WBC-D]	The white blood cell count measured from the WDF channel.
[TNC-D]	The total nucleated cell count (white blood cell count + nucleated red blood cell count) measured from the WDF channel.
[DLT-WBCD]	The ratio of WBC-D to WBC-C.
[iRBC-WDF#]*	The iRBC particle count measured from the WDF channel.
[Cell 1]	Total particle count measured in the WDF channel.
[Cell 2]	The particle count plotted in the WDF scattergram.
[Laser Current]	
[LD driver]	The current of the LD driver.

* The availability of analysis functions depends on your system configuration.

8.1.3 [HARDWARE] service data

To display the information below, touch the [Switch] button - [HARDWARE] on the toolbar.

[Unit Counter]	Displays the operation count of each unit. • [Total] shows the operation count of the overall analyzer. [Piercer] displays the operation count after piercer replacement.
[Temperature]	Displays the temperature of each unit. • [Environment Temp.] is the surrounding temperature.
[Pressure]	Displays pressure data at any set monitor timing.
[Laser]	The sum of the laser oscillation time is displayed.
[Aspiration Sensor]	Data used for monitoring of blood aspiration is displayed.
[RBC/HGB Drain Sensor]	Data used for monitoring of RBC/HGB analysis sample discharge is displayed.

8.1.4 [ADJUSTMENT] service data

A list of the items used for sensitivity adjustment appears in the ADJUSTMENT screen.

For items that are the same as in other screens, the same data is displayed.

To display the information below, touch the [Switch] button - [ADJUSTMENT] on the toolbar.

[WDF]	
[WDF-X]	The side scattered light intensity of the WBC area in the WDF scattergram.
[WDF-Y]	The fluorescence intensity of the WBC area in the WDF scattergram.
[WDF-Z]	The forward scattered light intensity of the WBC area in the WDF scattergram.
[LY-X]	The side scattered light intensity of the LYMPH area in the WDF scattergram.
[LY-Z]	The forward scattered light intensity of the LYMPH area in the WDF scattergram.

8.2 Checking research parameters

Research parameters are displayed on a gray background on the [Sample Explorer] screen and the [Data Browser] screen.



Information

Analysis results of research parameters are indicated by a gray background to distinguish them from reportable parameters to be reported. Analysis results of research parameters must not be used for the diagnosis of patients.

8.2.1 WBC research parameters

The WBC research parameters below can be set to be displayed.

TNC	The total nucleated cell count (white blood cell count + nucleated red blood cell count).
WBC-C	The total white blood cell count measured from the forward scattered light and the side scattered light of the WDF channel.
TNC-C	The total nucleated cell count (white blood cell count + nucleated cell count) measured from the forward scattered light and the side scattered light of the WDF channel.
WBC-D	The white blood cell count measured from the WDF channel.
TNC-D	The total nucleated cell count (white blood cell count + nucleated red blood cell count) measured from the WDF channel.
WBC-D&*	The particle count obtained by subtracting iRBC from WBC-D.
NRBC#	The nucleated red blood cell count.
NRBC%	The ratio of the nucleated red blood cell count.
NEUT#&	The particle count obtained by subtracting IG# from NEUT#.
NEUT%&	The ratio of the particle count obtained by subtracting IG# from NEUT# to the white blood cell count.
LYMP#&	The particle count obtained by subtracting HFLC# from LYMPH#.
LYMP%&	The ratio of the particle count obtained by subtracting HFLC# from LYMPH# to the white blood cell count.
HFLC#	The particle count of the upper LYMPH area in the WDF scattergram.
HFLC%	The ratio of the particle count of the upper LYMPH area in the WDF scattergram to the white blood cell count.
NE-SSC	The side scattered light intensity of the NEUT area in the WDF scattergram.
NE-SFL	The fluorescence intensity of the NEUT area in the WDF scattergram.
NE-FSC	The forward scattered light intensity of the NEUT area in the WDF scattergram.
LY-X	The side scattered light intensity of the LYMPH area in the WDF scattergram.
LY-Y	The fluorescence intensity of the LYMPH area in the WDF scattergram.
LY-Z	The forward scattered light intensity of the LYMPH area in the WDF scattergram.
MO-X	The side scattered light intensity of the MONO area in the WDF scattergram.
MO-Y	The fluorescence intensity of the MONO area in the WDF scattergram.
MO-Z	The forward scattered light intensity of the MONO area in the WDF scattergram.

* The availability of analysis functions depends on your system configuration.

NE-WX	The side scattered light distribution width index of the NEUT area in the WDF scattergram.
NE-WY	The fluorescence distribution width index of the NEUT area in the WDF scattergram.
NE-WZ	The forward scattered light distribution width index of the NEUT area in the WDF scattergram.
LY-WX	The side scattered light distribution width index of the LYMPH area in the WDF scattergram.
LY-WY	The fluorescence distribution width index of the LYMPH area in the WDF scattergram.
LY-WZ	The forward scattered light distribution width index of the LYMPH area in the WDF scattergram.
MO-WX	The side scattered light distribution width index of the MONO area in the WDF scattergram.
MO-WY	The fluorescence distribution width index of the MONO area in the WDF scattergram.
MO-WZ	The forward scattered light distribution width index of the MONO area in the WDF scattergram.

8.2.2 RBC/PLT research parameters

The RBC/PLT research parameters below can be set to be displayed.

PLT-I	The platelet count measured from the RBC/PLT channel (PLT distribution).
--------------	--------------------------------------------------------------------------

Index

A

Acceptable barcodes	64
Accessories.....	75
Accuracy	
[Pre-Dilution] mode	53
[Whole Blood] mode	51
Analyzer.....	29
Aspirated sample volume	
[Pre-Dilution] mode	42
[Whole Blood] mode	42
Automatically assigned numbers	65
Avoiding infection.....	18

B

Barcode labels	63
Barcodes	
Quality control (QC).....	65
Sample numbers	64

C

Calibrator	85
Carryover	
[Pre-Dilution] mode	55
[Whole Blood] mode	55
CELLCLEAN AUTO	83
CELLPACK DCL	78
CELLPACK DST	79
Checking service data.....	87
Computer viruses.....	20
Control blood.....	84

D

Dimensions and weight	
Analyzer.....	41
Monitor (XN-530).....	42
Disposal of materials.....	19

E

Electrical rating	
Analyzer.....	41
Monitor (XN-530).....	42
Electromagnetic compatibility (EMC).....	17

F

Fluorocell WDF	82
Functional descriptions	66

G

Grounding	38
-----------------	----

H

Hydraulic diagram	69
-------------------------	----

I

ID barcode specifications	64
Installation	37
Preparing for installation	37
Intended use	9
Introduction	7

L

Laser	19
Laser class	41
Linearity	
[Pre-Dilution] mode	47
[Whole Blood] mode	46
Lysercell WDF	81

M

Maintenance.....	19
Manuals.....	11
Markings on the instrument.....	21
Monitor	36

N

Noise level.....	41
------------------	----

O

Operating environment.....	41
Operators	20
Options.....	76
Overview of the system.....	9

P

Performance characteristics	
[Pre-Dilution] mode	45
[Whole Blood] mode	45
Precision (Repeatability)	
[Pre-Dilution] mode	49
[Whole Blood] mode	48

R

Reagents.....	18, 77
List	77
Reportable parameters	10
Reportable range and display range	
[Pre-Dilution] mode	44
[Whole Blood] mode	43

Research parameters.....	91	T	
RBC/PLT.....	92	Throughput	
WBC	91	[Pre-Dilution] mode	42
S		[Whole Blood] mode.....	42
Safety information	15	Trademarks	14
Safety standards	41	X	
Sample numbers	65	XN CAL	85
Sample tubes (XN-330).....	60	XN-L CHECK.....	84
Sample tubes (XN-530/XN-430)	60		
Sampler adapter.....	62		
Service data			
[ADJUSTMENT].....	90		
[HARDWARE].....	90		
[RBC/PLT].....	88		
[WDF].....	89		
Software specifications			
Data storage capacity	56		
Quality control (QC).....	56		
Specifications	41		
Accuracy	51		
Analyzer	41		
Aspirated sample volume	42		
Carryover	55		
Linearity	46		
Monitor (XN-530)	42		
Performance characteristics	45		
Precision (Repeatability).....	48		
Precision (Reproducibility).....	50		
Reportable range and display range.....	43		
Sample stability with time after blood			
collection	56		
Software specifications	56		
Throughput	42		
Storage conditions			
Analyzer	41		
Monitor (XN-530)	42		
SULFOLYSER.....	80		
Supplies	75		
Symbols used in the manuals	12		
System limitations	57		